


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111618\
Data File : VV008573.D
Acq On : 16 Nov 2018 09:04
Operator : SY/MD
Sample : BFB47
Misc : 5.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB47

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111518WMA.M
Title : VOC Analysis
Last Update : Fri Nov 16 23:18:19 2018

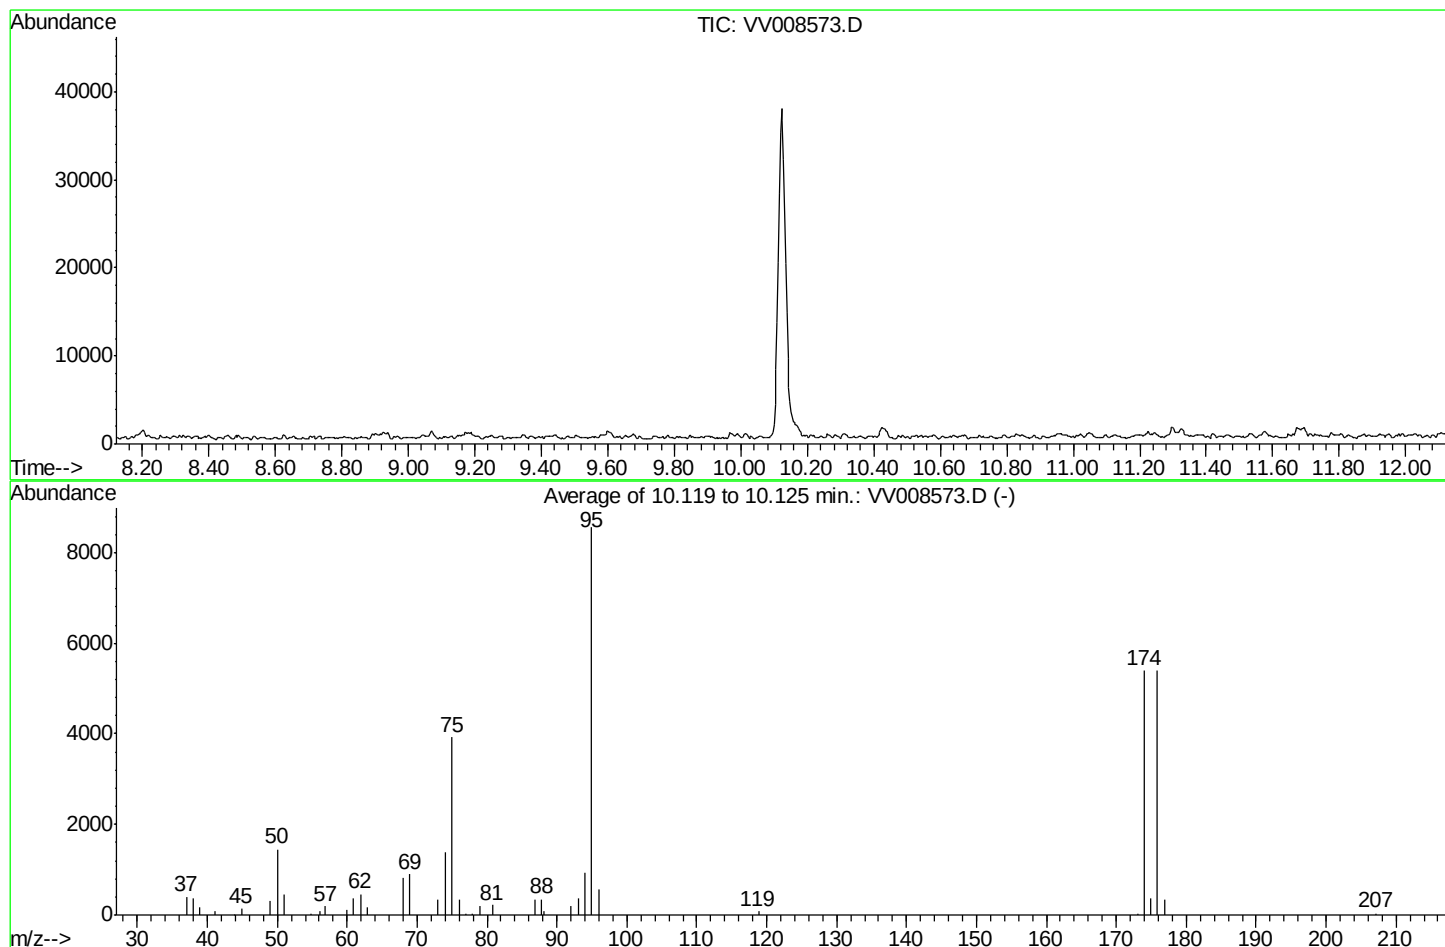

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2798

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	1456	PASS
75	95	30	80	45.9	3928	PASS
95	95	100	100	100.0	8559	PASS
96	95	5	9	6.8	579	PASS
173	174	0.00	2	0.6	35	PASS
174	95	50	120	63.0	5391	PASS
175	174	5	9	6.7	362	PASS
176	174	95	101	99.9	5385	PASS
177	176	5	9	6.4	342	PASS

m/z	Abundance
39.90	312.0
43.90	399.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
37.00	411.0
37.90	355.0
38.90	200.0
39.90	180.0
41.10	146.0
44.00	438.0
44.80	135.0
48.90	318.0
50.00	1384.0
50.90	467.0
54.90	123.0
56.90	177.0
59.90	106.0
60.90	362.0
61.90	480.0
62.90	175.0
68.00	736.0
69.00	903.0
72.90	301.0
74.00	1321.0
75.00	3954.0
76.00	338.0
77.00	103.0
78.90	256.0
80.80	224.0
86.80	341.0
87.90	406.0
91.90	176.0
93.00	401.0
94.00	1000.0
95.00	8533.0
96.00	581.0
174.00	5541.0
174.90	296.0
175.90	5445.0
176.90	327.0
207.20	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
37.00	442.0
37.90	386.0
38.80	161.0
40.00	222.0
41.10	136.0
44.00	387.0
44.90	150.0
48.90	330.0
50.00	1526.0
50.90	459.0
56.10	112.0
56.80	207.0
59.90	118.0
60.90	388.0
62.00	497.0
62.90	176.0
68.00	862.0
69.00	928.0
72.90	348.0
74.00	1449.0
75.00	4031.0
76.00	345.0
78.90	207.0
80.80	225.0
86.90	337.0
87.80	376.0
91.90	218.0
93.00	393.0
93.90	985.0
95.00	9003.0
96.00	599.0
118.80	108.0
173.10	107.0
174.00	5639.0
174.90	369.0
175.90	5597.0
176.90	353.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47

m/z	Abundance
37.00	370.0
37.90	383.0
38.90	127.0
40.00	279.0
43.90	375.0
44.90	137.0
48.90	311.0
50.00	1458.0
50.90	451.0
56.10	112.0
56.80	193.0
59.90	100.0
60.90	389.0
62.00	385.0
62.90	181.0
68.10	871.0
68.90	849.0
72.90	377.0
74.00	1374.0
75.00	3799.0
76.00	327.0
77.80	119.0
79.00	163.0
80.80	199.0
86.90	317.0
87.80	279.0
88.10	276.0
91.90	224.0
93.00	349.0
93.90	847.0
95.00	8143.0
96.00	557.0
118.80	146.0
174.00	4994.0
174.90	422.0
175.90	5113.0
176.90	346.0

Instrument :
MSVOA_V
ClientSampleId :
BFB47