


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
Data File : VV023540.D
Acq On : 16 Nov 2021 17:37
Operator : SY/MD
Sample : M4643-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
Client Sampled :
GB8K1

Quant Time: Nov 17 02:00:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 17 00:48:57 2021
Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/17/2021
Supervised By : Mahesh Dadoda 11/18/2021

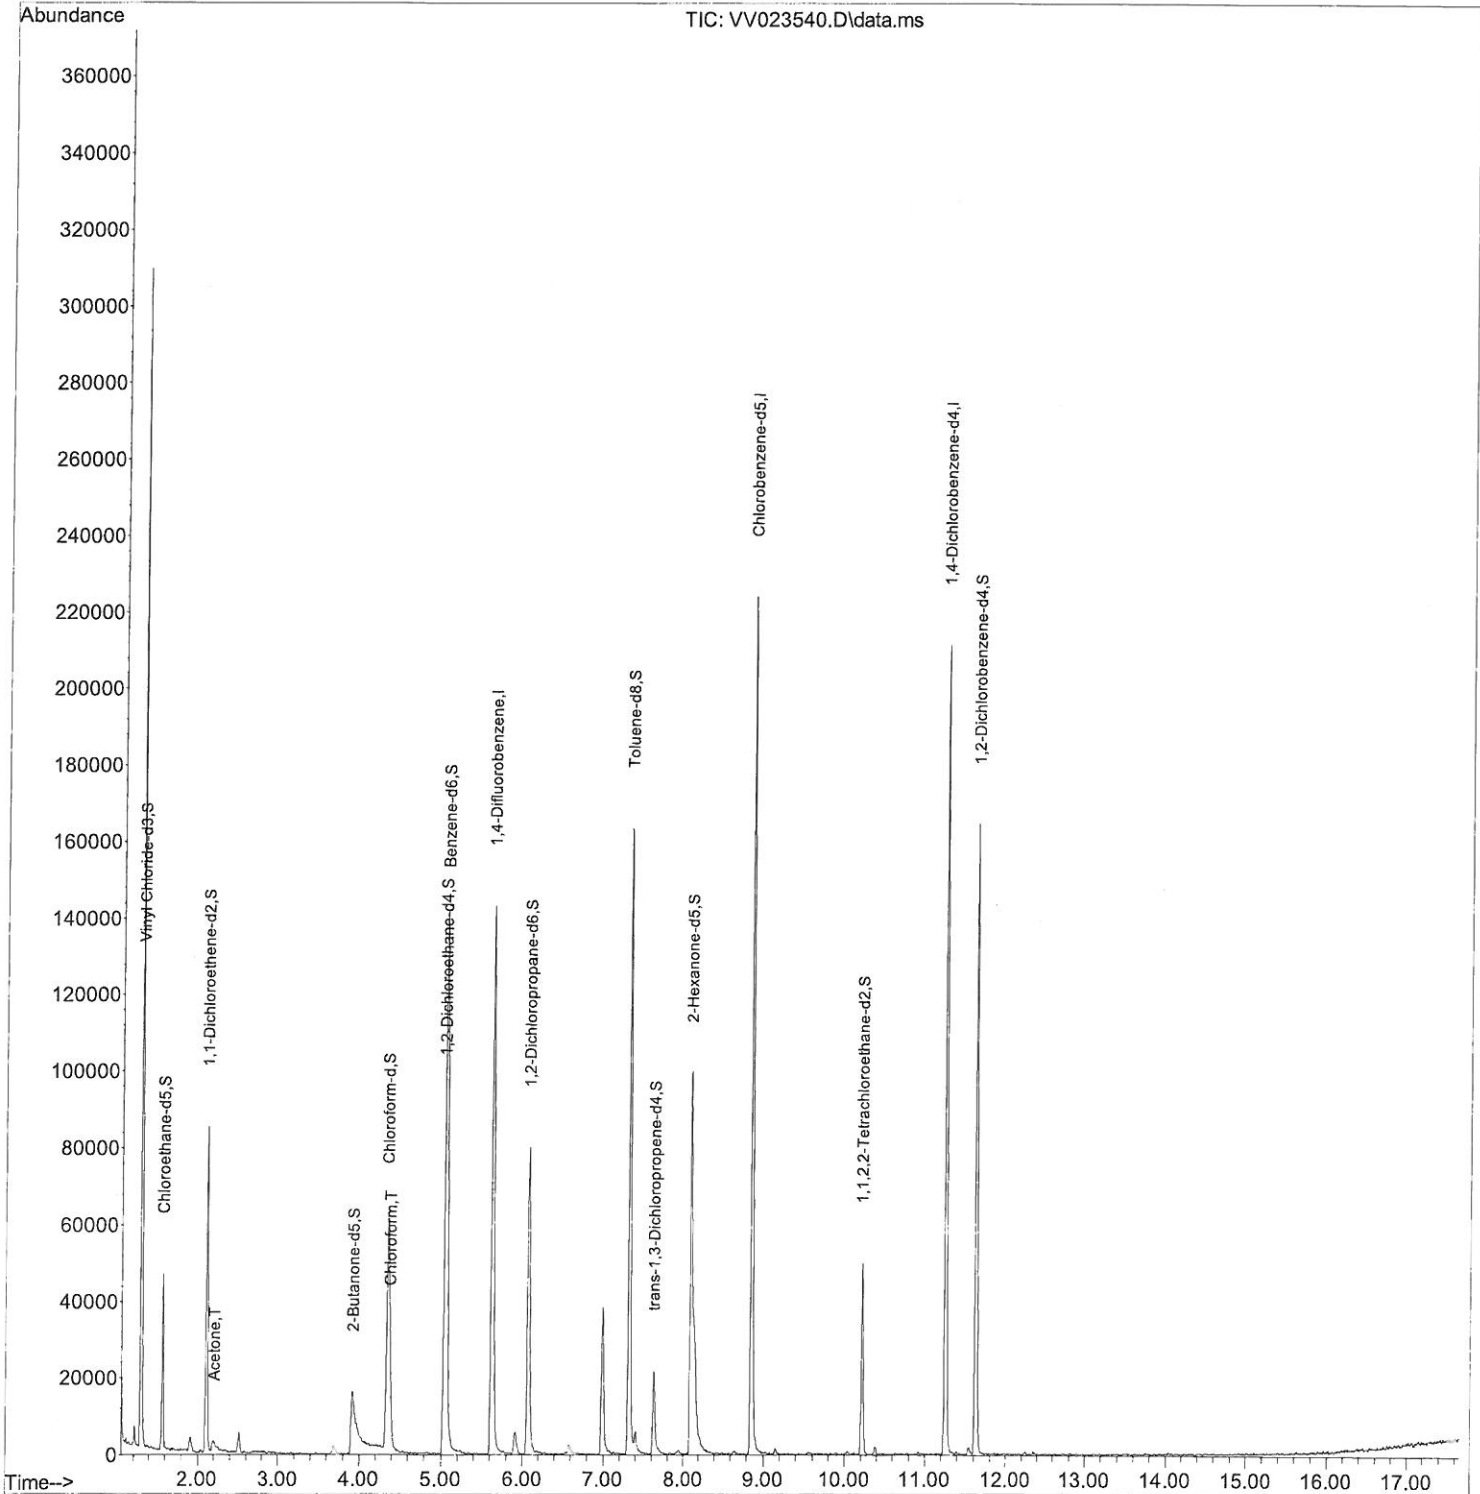

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
 Data File : VV023540.D
 Acq On : 16 Nov 2021 17:37
 Operator : SY/MD
 Sample : M4643-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 GB8K1

Quant Time: Nov 17 00:54:08 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 17 00:48:57 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/17/2021
 Supervised By : Mahesh Dadoda 11/18/2021

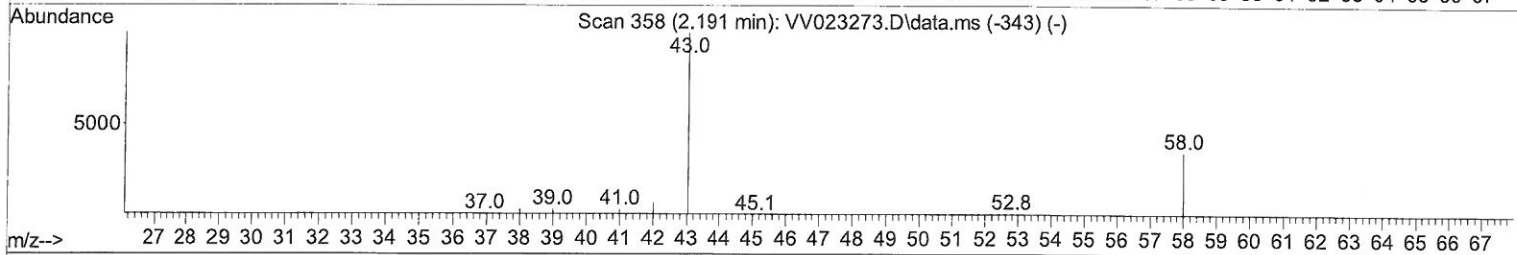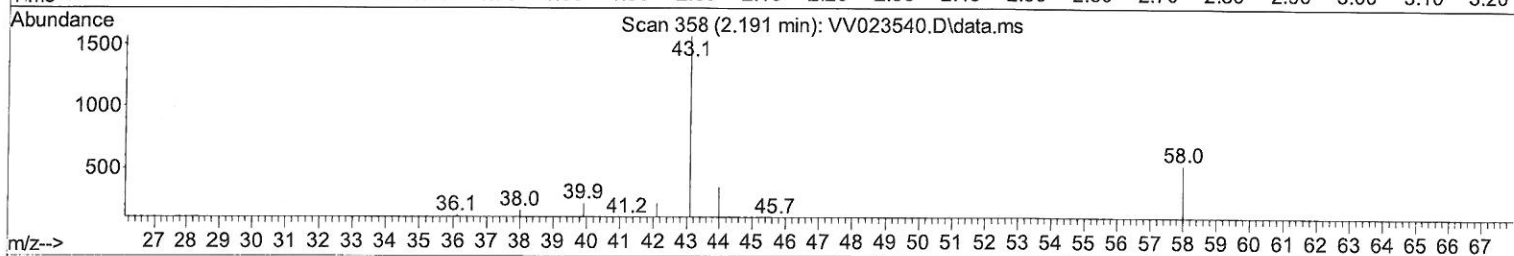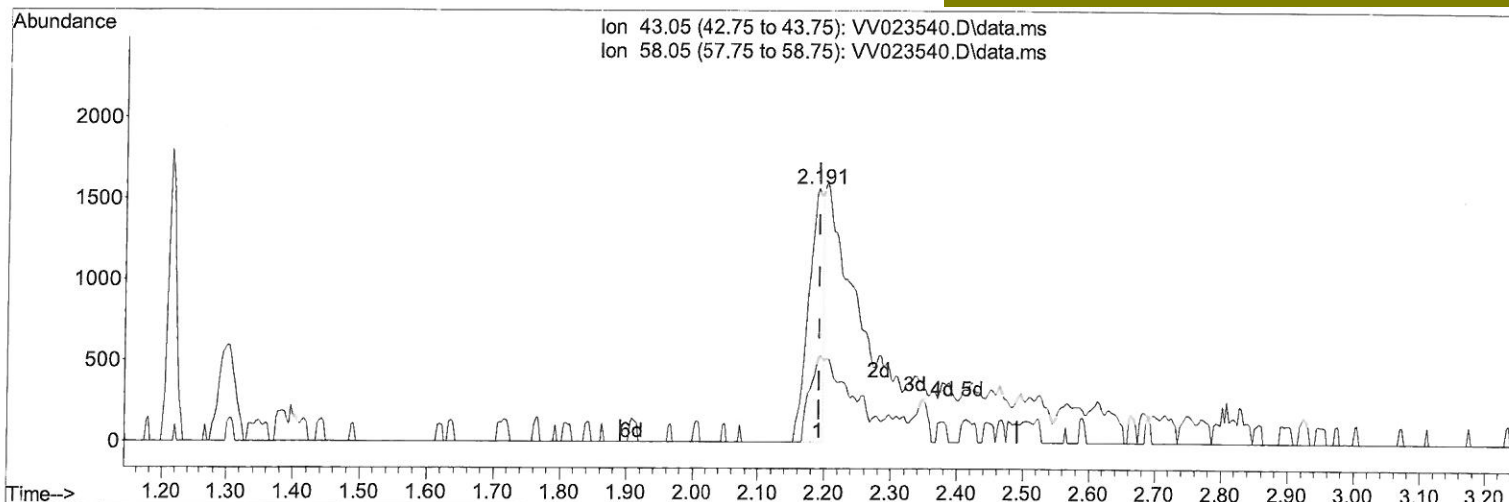

TIC: VV023540.D\data.ms

(13) Acetone (T)

2.191min (-0.000) 2.90 ug/L

response 2453

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	54.71
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
 Data File : VV023540.D
 Acq On : 16 Nov 2021 17:37
 Operator : SY/MD
 Sample : M4643-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 GB8K1

Manual Integrations APPROVED

Reviewed By : John Carlone 11/17/2021
 Supervised By : Mahesh Dadoda 11/18/2021

Quant Time: Nov 17 02:00:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 17 00:48:57 2021
 Response via : Initial Calibration

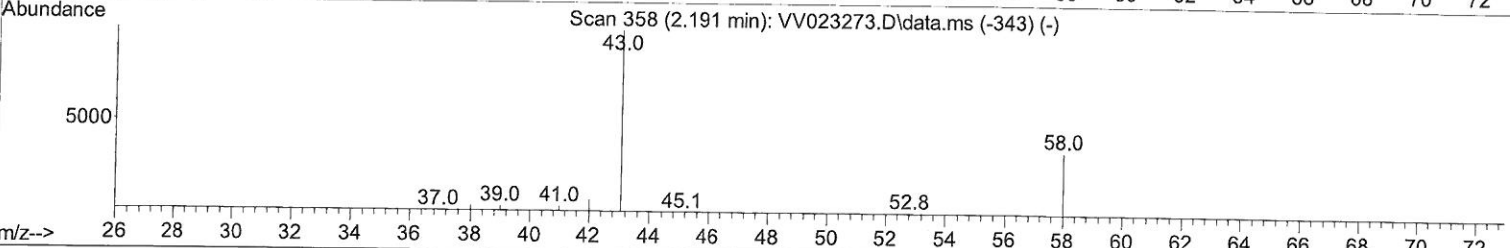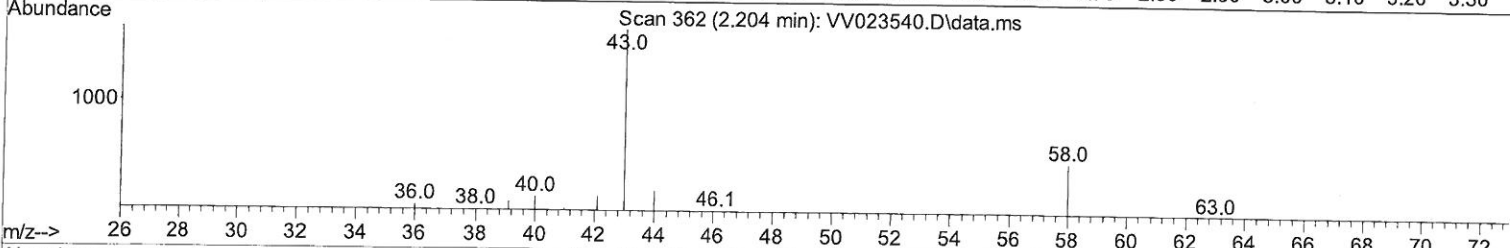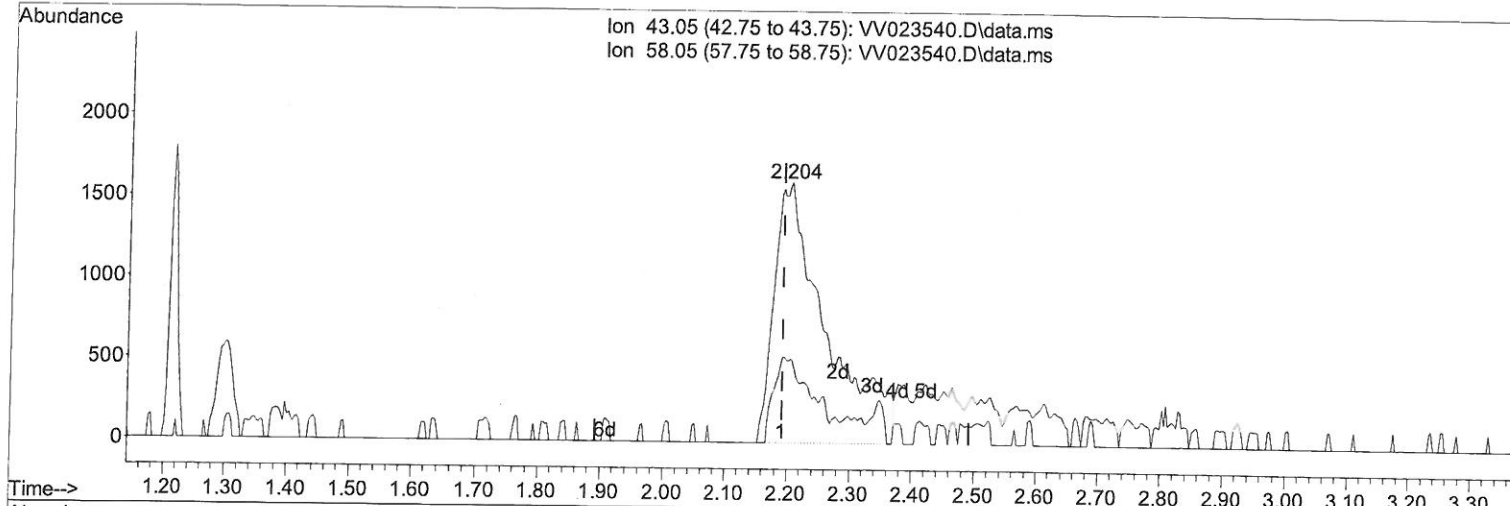

TIC: VV023540.D\data.ms

(13) Acetone (T)

2.204min (+ 0.013) 10.94 ug/L m *MD*
11/26/21

response 9272

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	14.47
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
 Data File : VV023540.D
 Acq On : 16 Nov 2021 17:37
 Operator : SY/MD
 Sample : M4643-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 Client Sampled :
 GB8K1

Quant Time: Nov 17 02:00:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 17 00:48:57 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : John Carlone 11/17/2021
 Supervised By : Mahesh Dadoda 11/18/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	128483	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	129022	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	56573	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	31175	3.873	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	77.400%		
7) Chloroethane-d5	1.568	69	26587	4.053	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	81.000%		
11) 1,1-Dichloroethene-d2	2.108	63	43383	2.879	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	57.600%#		
20) 2-Butanone-d5	3.918	46	38200	27.548	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	55.100%		
24) Chloroform-d	4.349	84	61491	3.585	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	71.600%		
26) 1,2-Dichloroethane-d4	5.034	65	32836	4.257	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	85.200%		
32) Benzene-d6	5.053	84	128196	3.872	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	77.400%		
36) 1,2-Dichloropropane-d6	6.072	67	38834	3.985	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	79.800%		
41) Toluene-d8	7.316	98	109758	3.538	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	70.800%		
43) trans-1,3-Dichloroprop...	7.625	79	13816	3.739	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	74.800%		
46) 2-Hexanone-d5	8.091	63	42668	31.384	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	62.760%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	24247	3.460	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	69.200%		
66) 1,2-Dichlorobenzene-d4	11.625	152	44002	4.671	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	93.400%		
Target Compounds						
13) Acetone	2.204	43	9272m	10.943	ug/L	Qvalue
25) Chloroform	4.378	83	10921	0.644	ug/L	92

MD
 11/26/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed