


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
Data File : VV023551.D
Acq On : 16 Nov 2021 22:22
Operator : SY/MD
Sample : M4627-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4630

Manual IntegrationsAPPROVED

Quant Time: Nov 17 03:40:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 17 02:49:39 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/17/2021
Supervised By :Mahesh Dadoda 11/18/2021

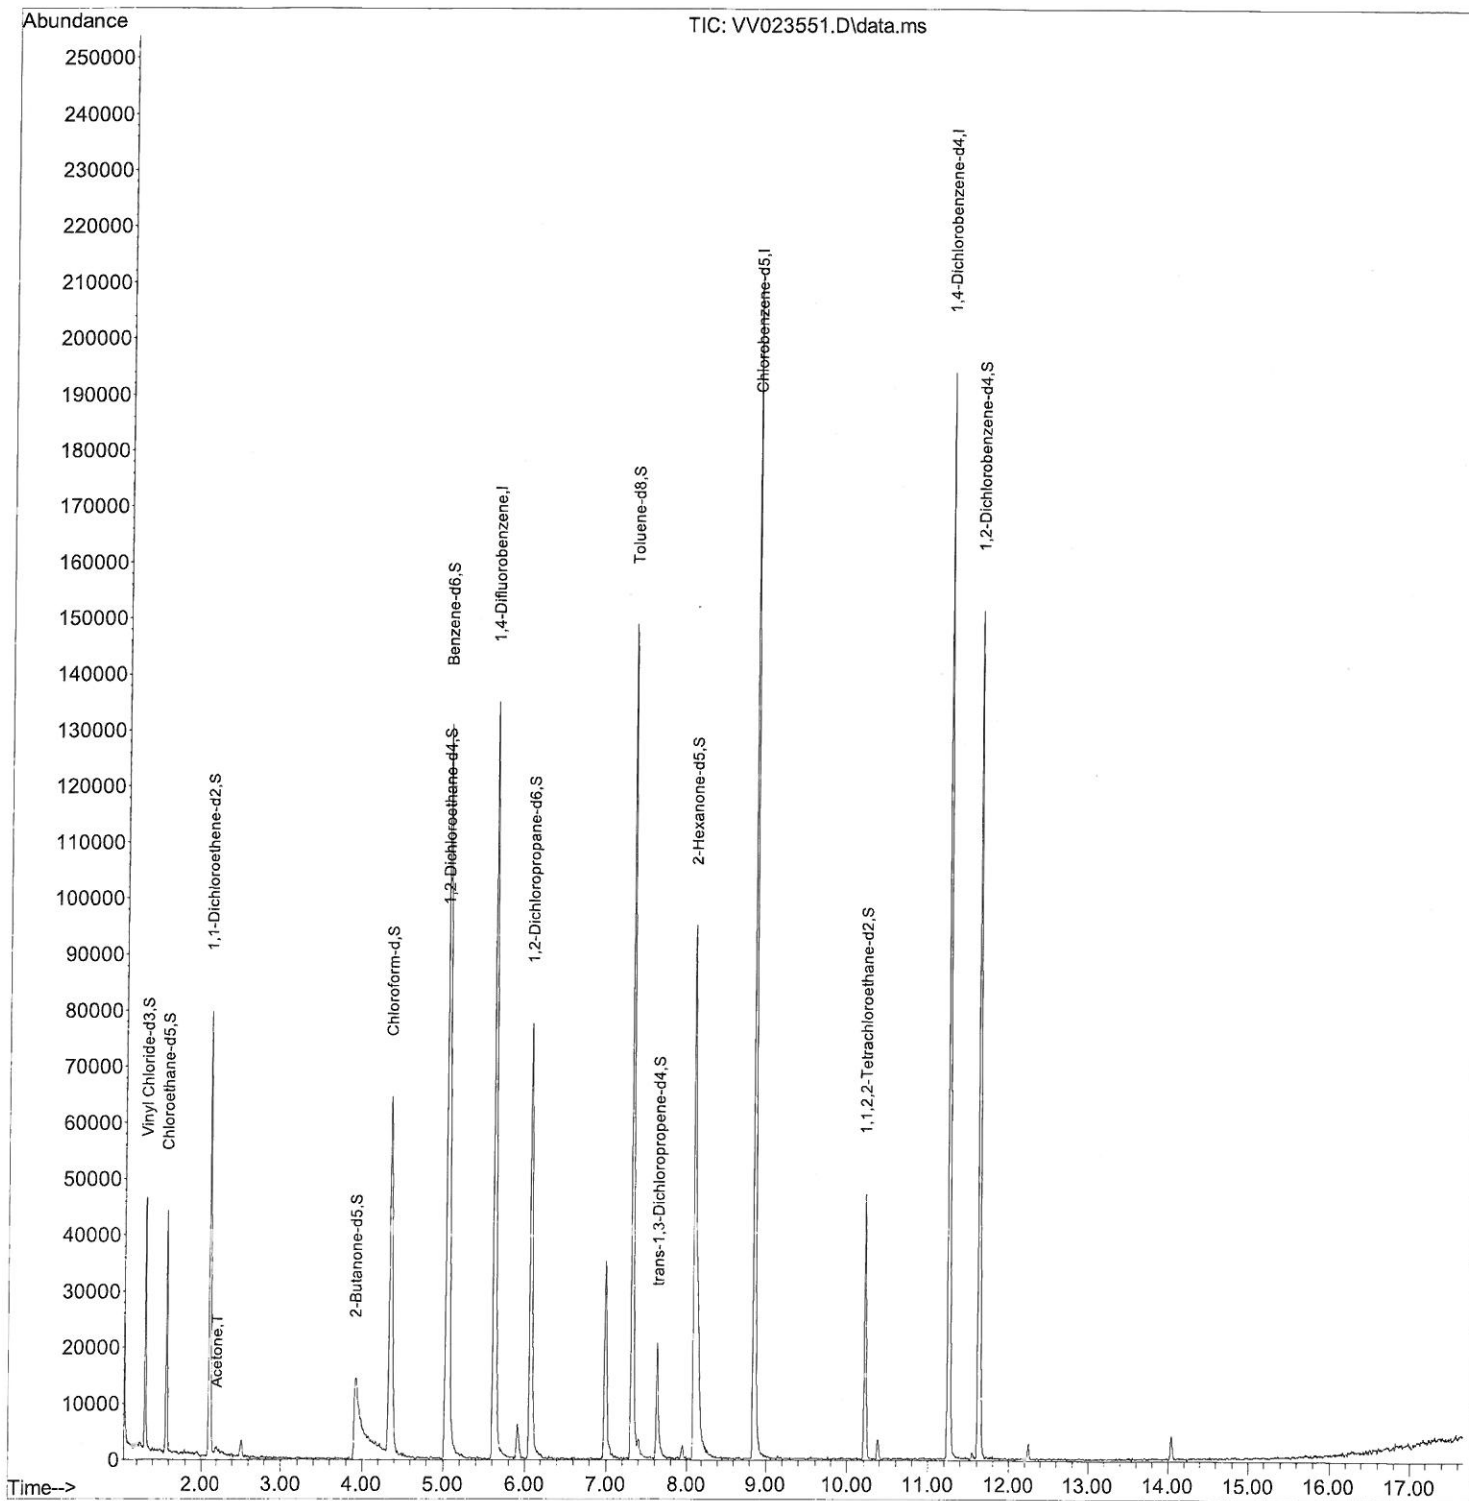

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
 Data File : VV023551.D
 Acq On : 16 Nov 2021 22:22
 Operator : SY/MD
 Sample : M4627-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4630

Manual IntegrationsAPPROVED

Quant Time: Nov 17 03:40:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 17 02:49:39 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/17/2021
 Supervised By :Mahesh Dadoda 11/18/2021

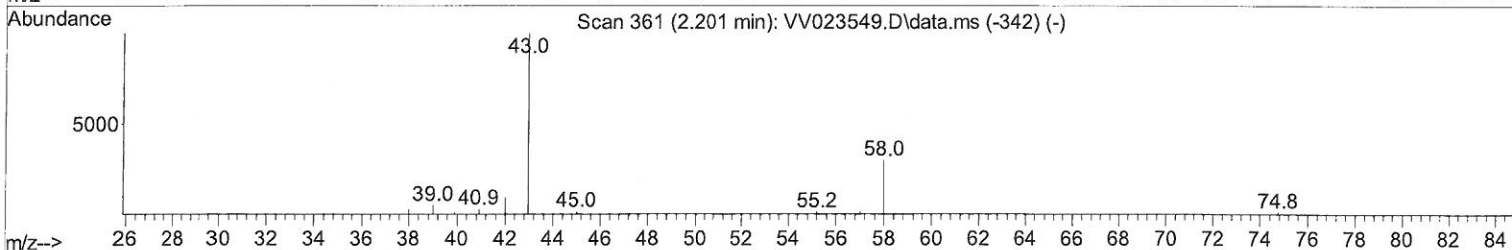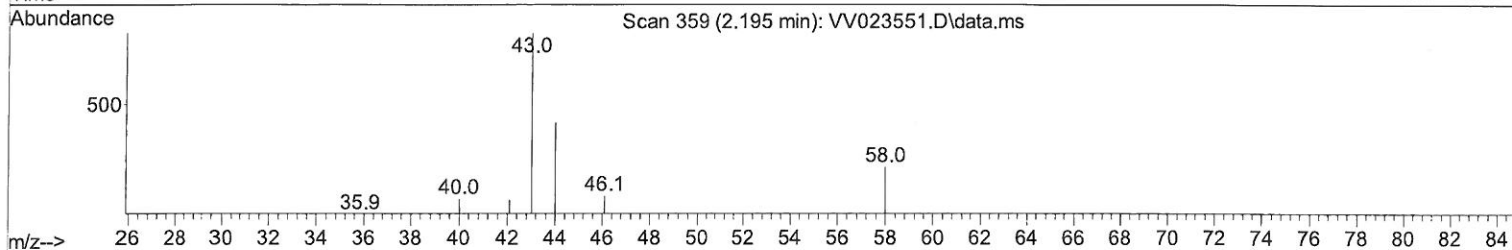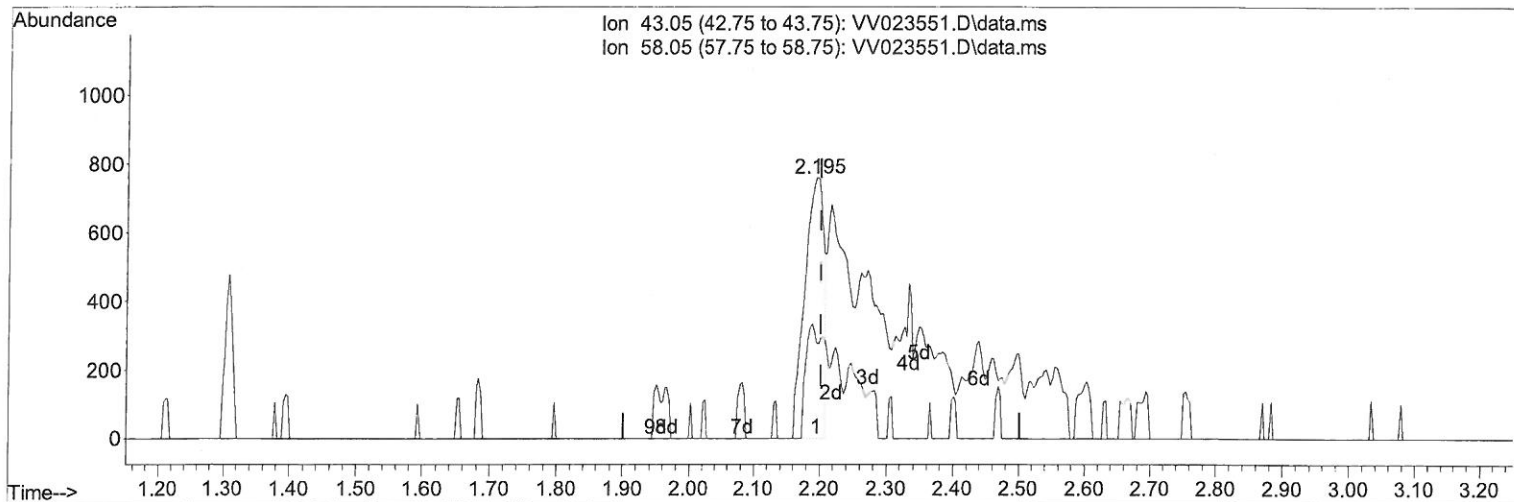

TIC: VV023551.D\data.ms

(13) Acetone (T)

2.195min (-0.006) 1.92 ug/L

response 1521

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	27.74
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
 Data File : VV023551.D
 Acq On : 16 Nov 2021 22:22
 Operator : SY/MD
 Sample : M4627-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4630

Manual IntegrationsAPPROVED

Quant Time: Nov 17 03:40:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 17 02:49:39 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/17/2021
 Supervised By :Mahesh Dadoda 11/18/2021

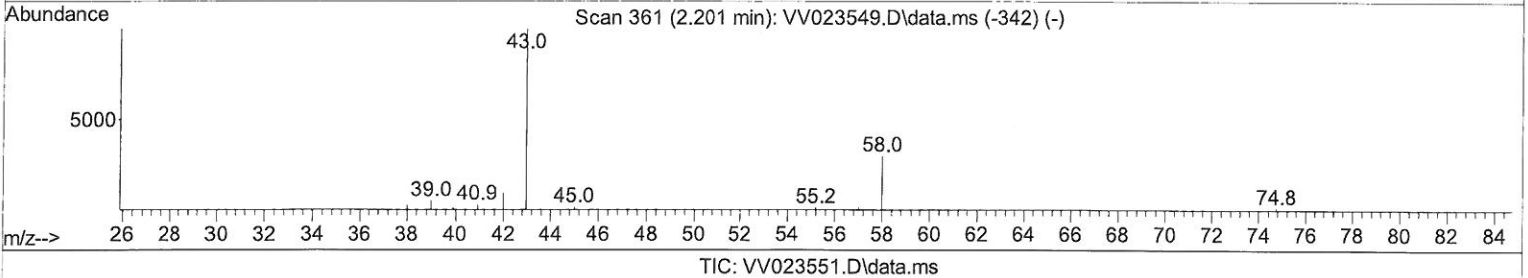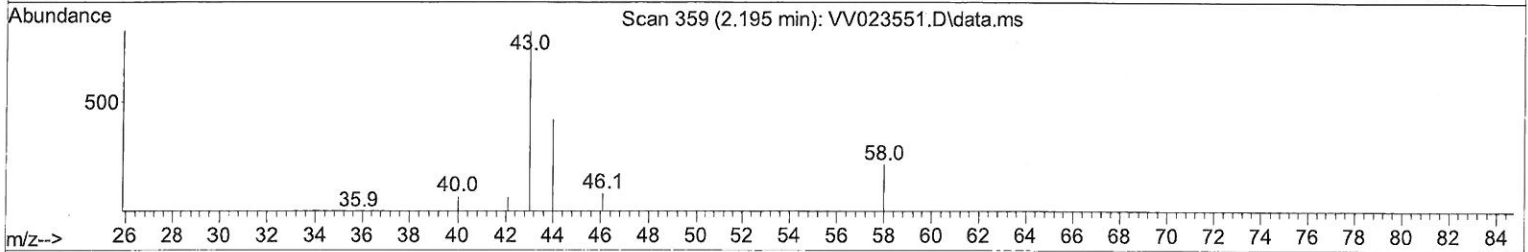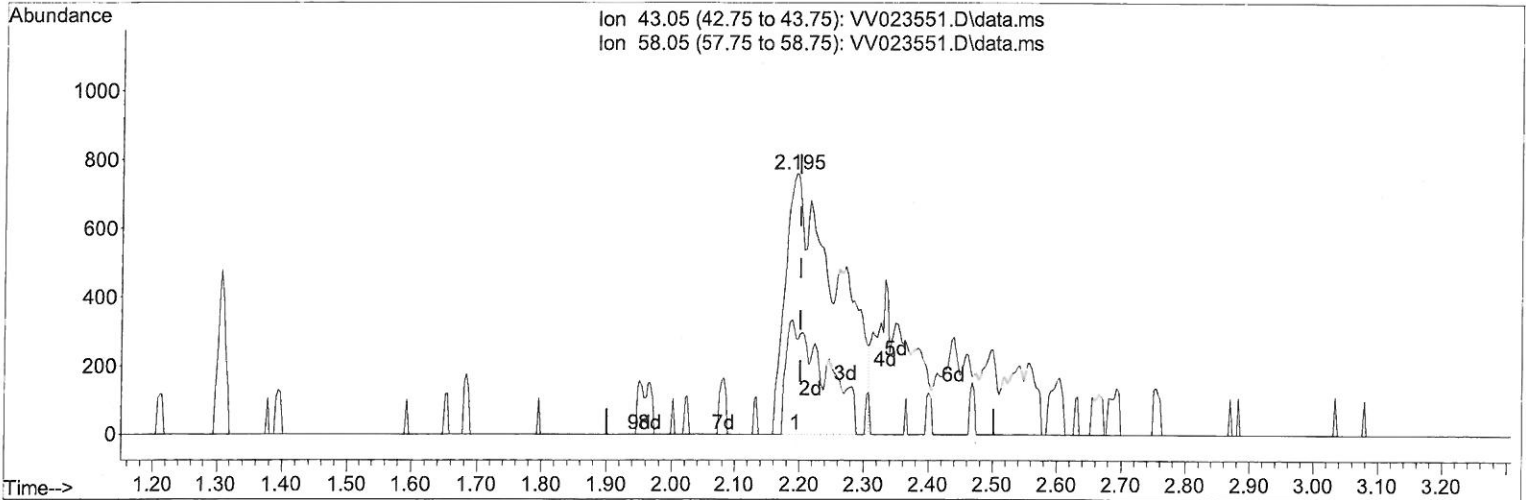

(13) Acetone (T)

2.195min (-0.006) 5.37 ug/L m

response 4249

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	27.70	9.93
0.00	0.00	0.00
0.00	0.00	0.00

MD
 11/26/21

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
Data File : VV023551.D
Acq On : 16 Nov 2021 22:22
Operator : SY/MD
Sample : M4627-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 32 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4630

Manual IntegrationsAPPROVED

Quant Time: Nov 17 03:40:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Wed Nov 17 02:49:39 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/17/2021
Supervised By :Mahesh Dadoda 11/18/2021

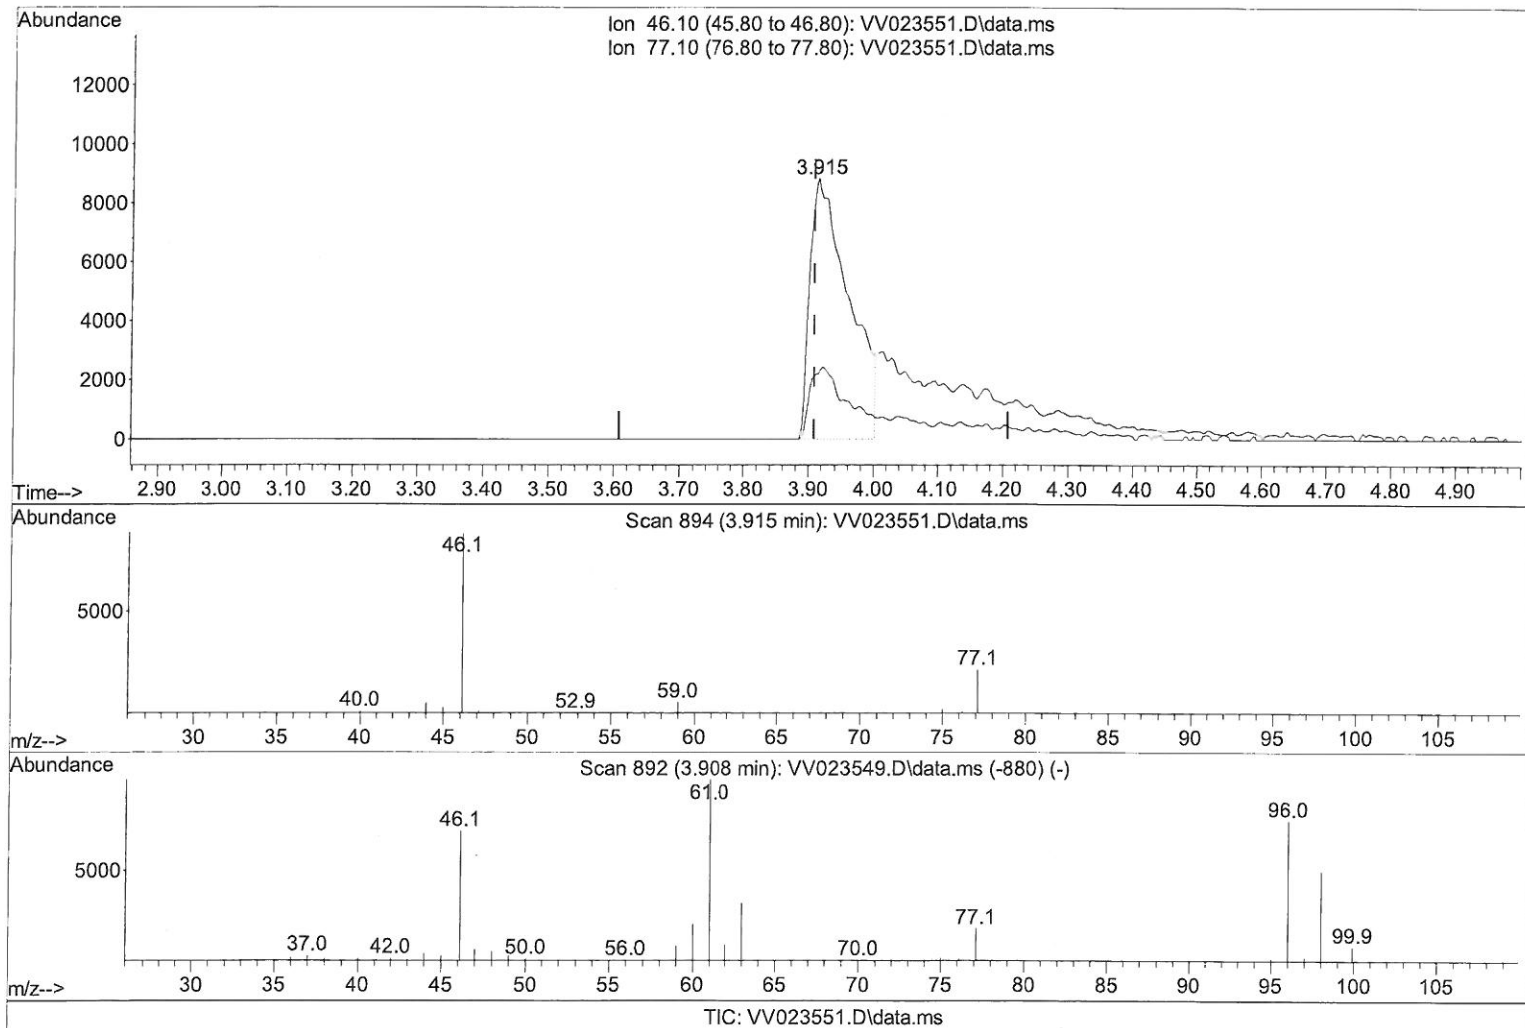

(20) 2-Butanone-d5 (S)

3.915min (+ 0.006) 28.24 ug/L

response 36587

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	22.39
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
 Data File : VV023551.D
 Acq On : 16 Nov 2021 22:22
 Operator : SY/MD
 Sample : M4627-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4630

Manual IntegrationsAPPROVED

Quant Time: Nov 17 03:40:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 17 02:49:39 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/17/2021
 Supervised By :Mahesh Dadoda 11/18/2021

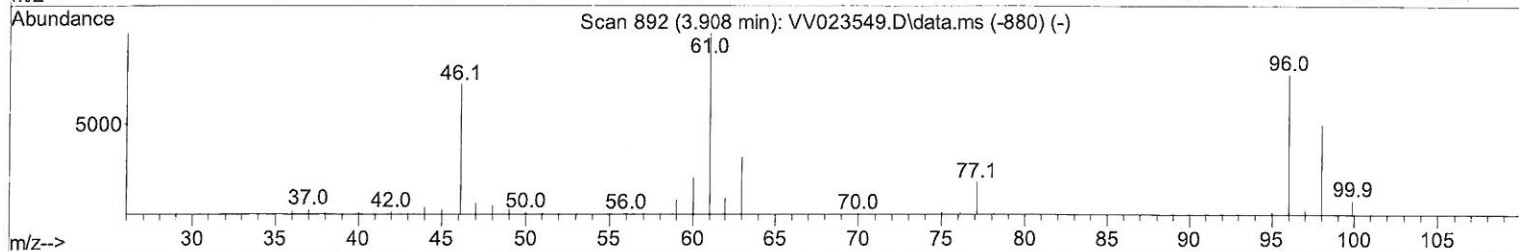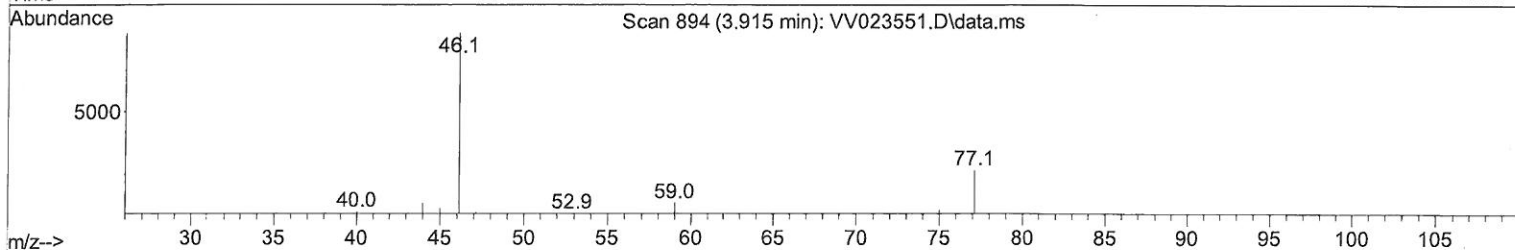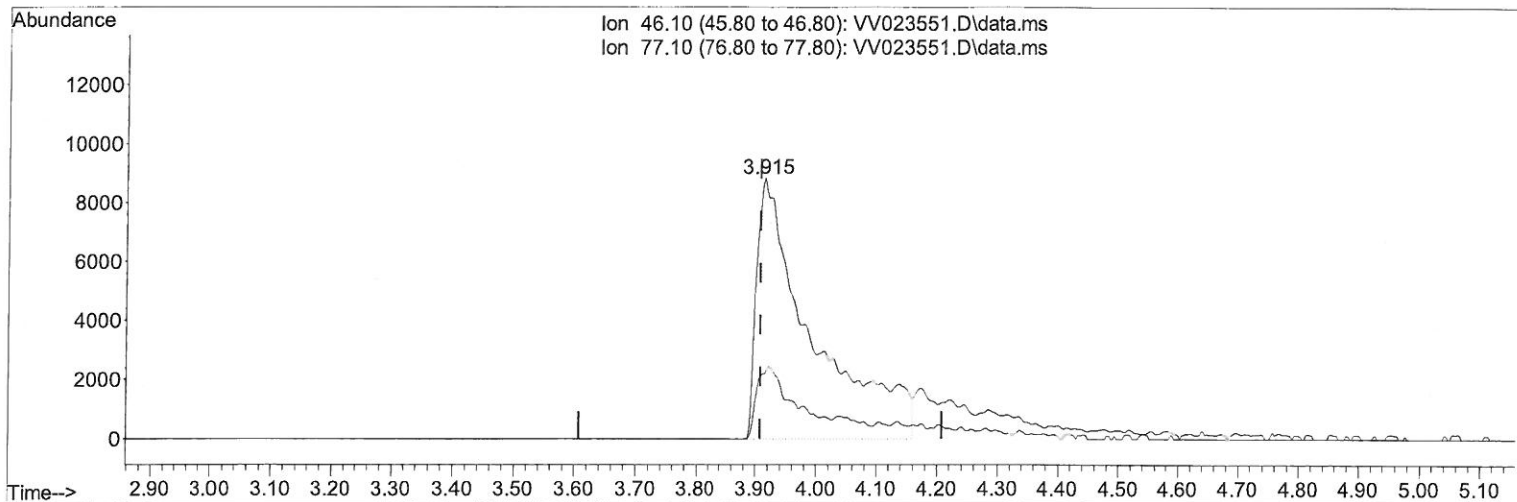

TIC: VV023551.D\data.ms

(20) 2-Butanone-d5 (S)

3.915min (+ 0.006) 43.18 ug/L m

response 55931

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	14.64#
0.00	0.00	0.00
0.00	0.00	0.00

MD
 11/26/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
 Data File : VV023551.D
 Acq On : 16 Nov 2021 22:22
 Operator : SY/MD
 Sample : M4627-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4630

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 11/17/2021
 Supervised By : Mahesh Dadoda 11/18/2021

Quant Time: Nov 17 03:40:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Wed Nov 17 02:49:39 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	120025	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.854	117	119982	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	52210	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	26885	3.576	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery	=	71.600%	
7) Chloroethane-d5	1.568	69	25340	4.135	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery	=	82.600%	
11) 1,1-Dichloroethene-d2	2.108	63	40577	2.883	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery	=	57.600%#	
20) 2-Butanone-d5	3.915	46	55931m	43.176	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery	=	86.360%	
24) Chloroform-d	4.349	84	64408	4.019	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery	=	80.400%	
26) 1,2-Dichloroethane-d4	5.034	65	31157	4.324	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery	=	86.400%	
32) Benzene-d6	5.050	84	119030	3.866	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery	=	77.400%	
36) 1,2-Dichloropropane-d6	6.069	67	38337	4.230	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery	=	84.600%	
41) Toluene-d8	7.317	98	99898	3.463	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery	=	69.200%#	
43) trans-1,3-Dichloroprop...	7.629	79	12806	3.727	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery	=	74.600%	
46) 2-Hexanone-d5	8.095	63	40092	31.711	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery	=	63.420%	
56) 1,1,2,2-Tetrachloroeth...	10.217	84	22438	3.443	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery	=	68.800%	
66) 1,2-Dichlorobenzene-d4	11.625	152	39939	4.594	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery	=	91.800%	
Target Compounds						
13) Acetone	2.195	43	4249m	5.368	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed