

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
 Data File : VV023534.D
 Acq On : 16 Nov 2021 15:10
 Operator : SY/MD
 Sample : M4616-12DL 10X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1Y5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023534.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.134	24	29	36	rVB2	6988	6546	1.11%	0.147%
2	1.201	44	50	60	rBV	160258	140307	23.79%	3.156%
3	1.307	76	83	96	rVB	52910	54978	9.32%	1.237%
4	1.568	156	164	174	rBV	46034	53168	9.01%	1.196%
5	2.108	321	332	351	rBV2	97156	150061	25.44%	3.375%
6	2.510	446	457	471	rBV2	14860	26009	4.41%	0.585%
7	3.908	880	892	924	rBV2	29218	119832	20.32%	2.695%
8	4.352	1014	1030	1056	rBV	67681	172123	29.18%	3.871%
9	5.050	1230	1247	1275	rBV3	147723	369568	62.66%	8.312%
10	5.619	1410	1424	1444	rBV	139760	284272	48.20%	6.394%
11	5.915	1503	1516	1548	rBV	295564	589782	100.00%	13.266%
12	6.069	1552	1564	1591	rVB2	84634	175074	29.68%	3.938%
13	6.989	1840	1850	1871	rBV	41168	77464	13.13%	1.742%
14	7.317	1938	1952	1973	rBV	176372	311767	52.86%	7.012%
15	7.625	2038	2048	2065	rBV2	23286	43229	7.33%	0.972%
16	7.976	2139	2157	2175	rBV	332795	561517	95.21%	12.630%
17	8.091	2184	2193	2232	rBV3	131416	291617	49.44%	6.559%
18	8.853	2418	2430	2453	rBV	214618	352229	59.72%	7.922%
19	10.217	2844	2854	2866	rBV2	54261	86406	14.65%	1.943%
20	11.249	3165	3175	3193	rBV	200257	314138	53.26%	7.066%
21	11.625	3278	3292	3309	rBV	167099	265884	45.08%	5.980%




Sum of corrected areas: 4445971

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
Data File : VV023534.D
Acq On : 16 Nov 2021 15:10
Operator : SY/MD
Sample : M4616-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

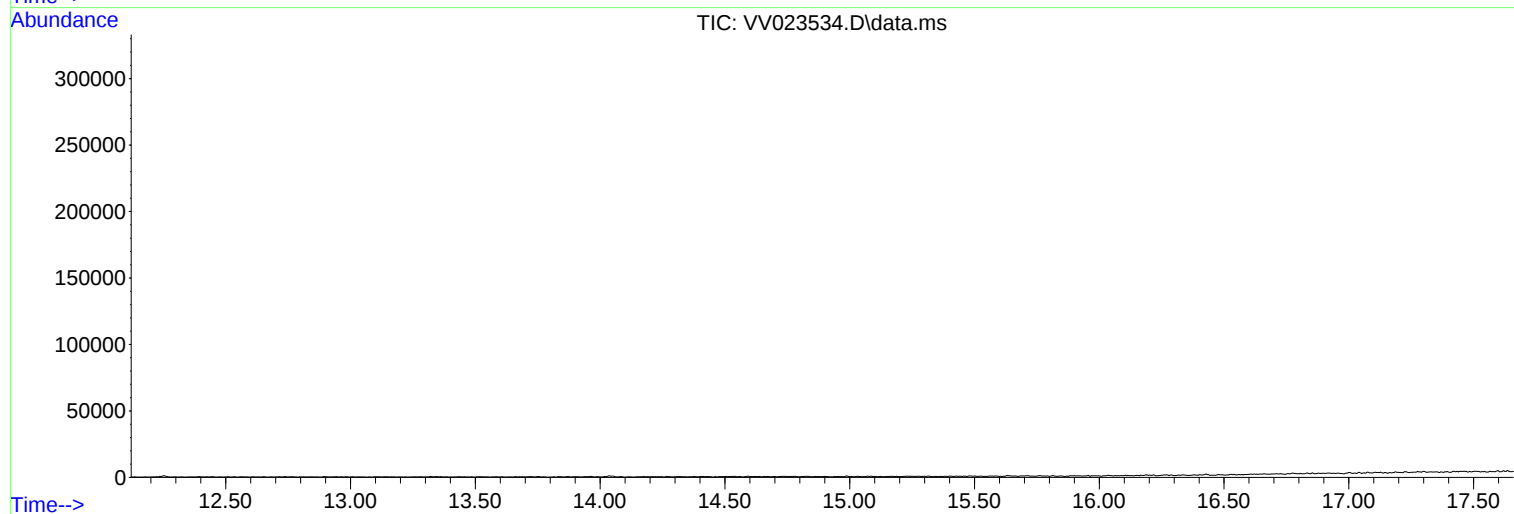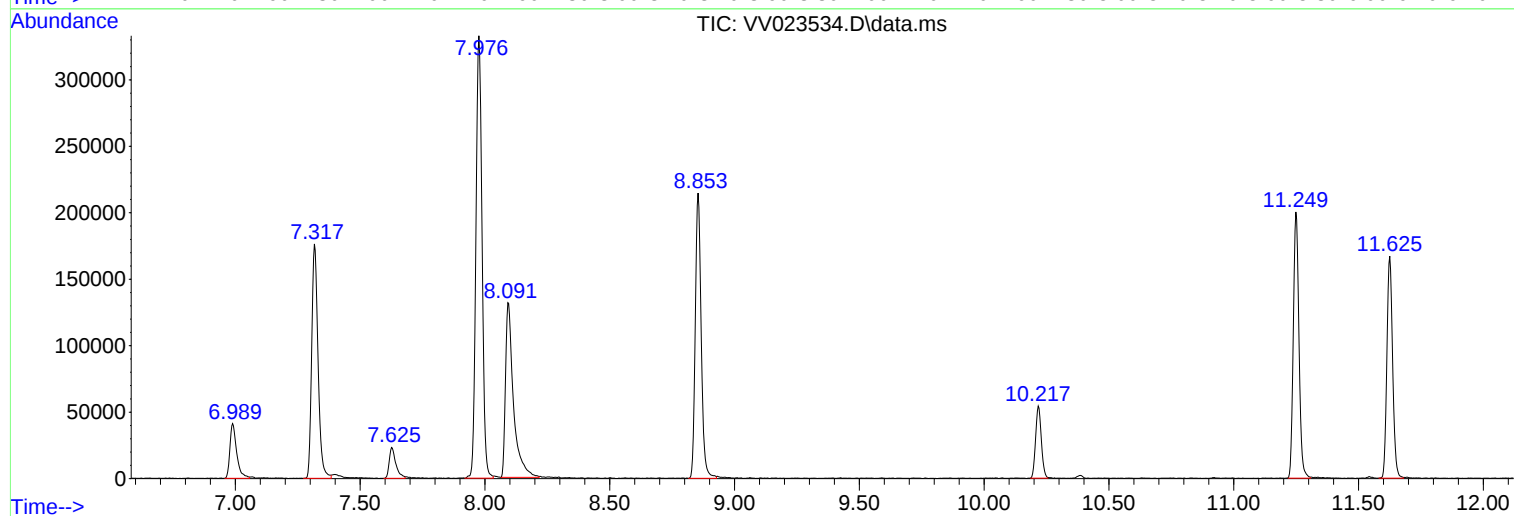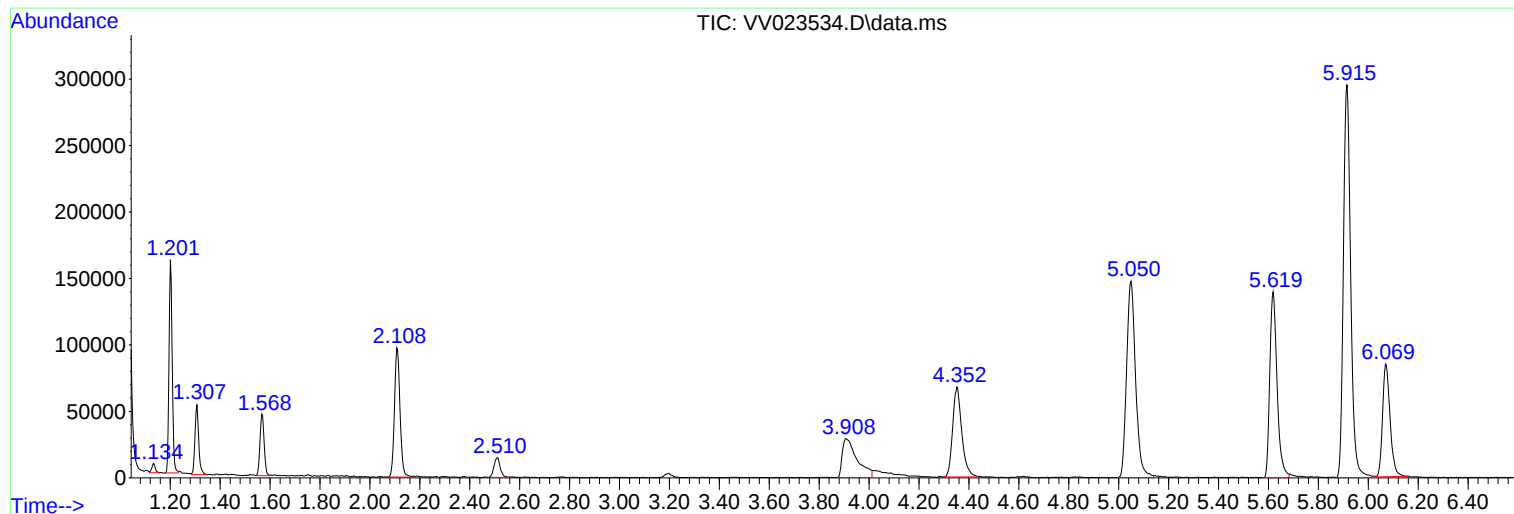

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
Data File : VV023534.D
Acq On : 16 Nov 2021 15:10
Operator : SY/MD
Sample : M4616-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y5DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	2.47 ug/L	140307	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
3			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4
4			Cyanogen chloride	61	CClN	000506-77-4	4
5			Trifluoroguanidine	113	CH2F3N3	037950-72-4	4

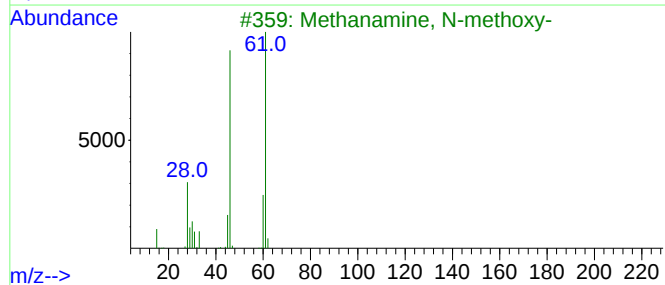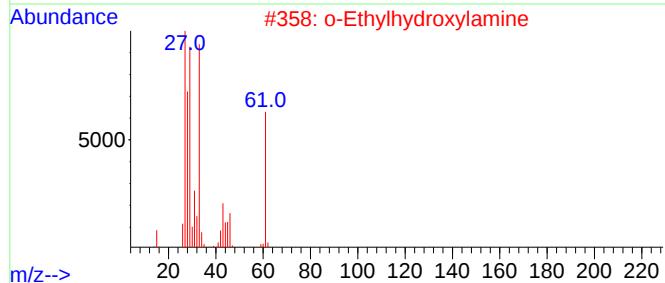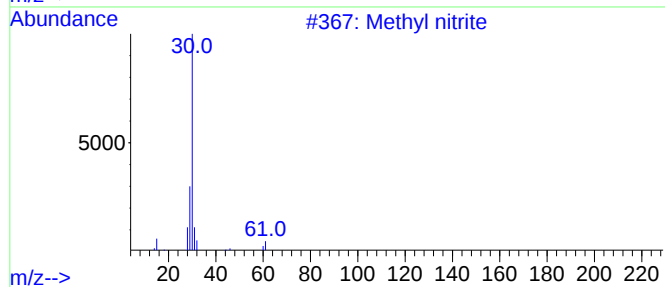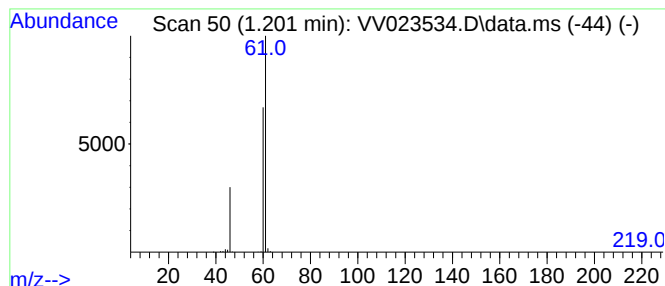

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
Data File : VV023534.D
Acq On : 16 Nov 2021 15:10
Operator : SY/MD
Sample : M4616-12DL 10X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	2.5	ug/L	140307	1	5.619	284272	5.0