


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111621\
Data File : VV023521.D
Acq On : 16 Nov 2021 09:34
Operator : SY/MD
Sample : BFB235
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB235

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Nov 18 00:20:29 2021

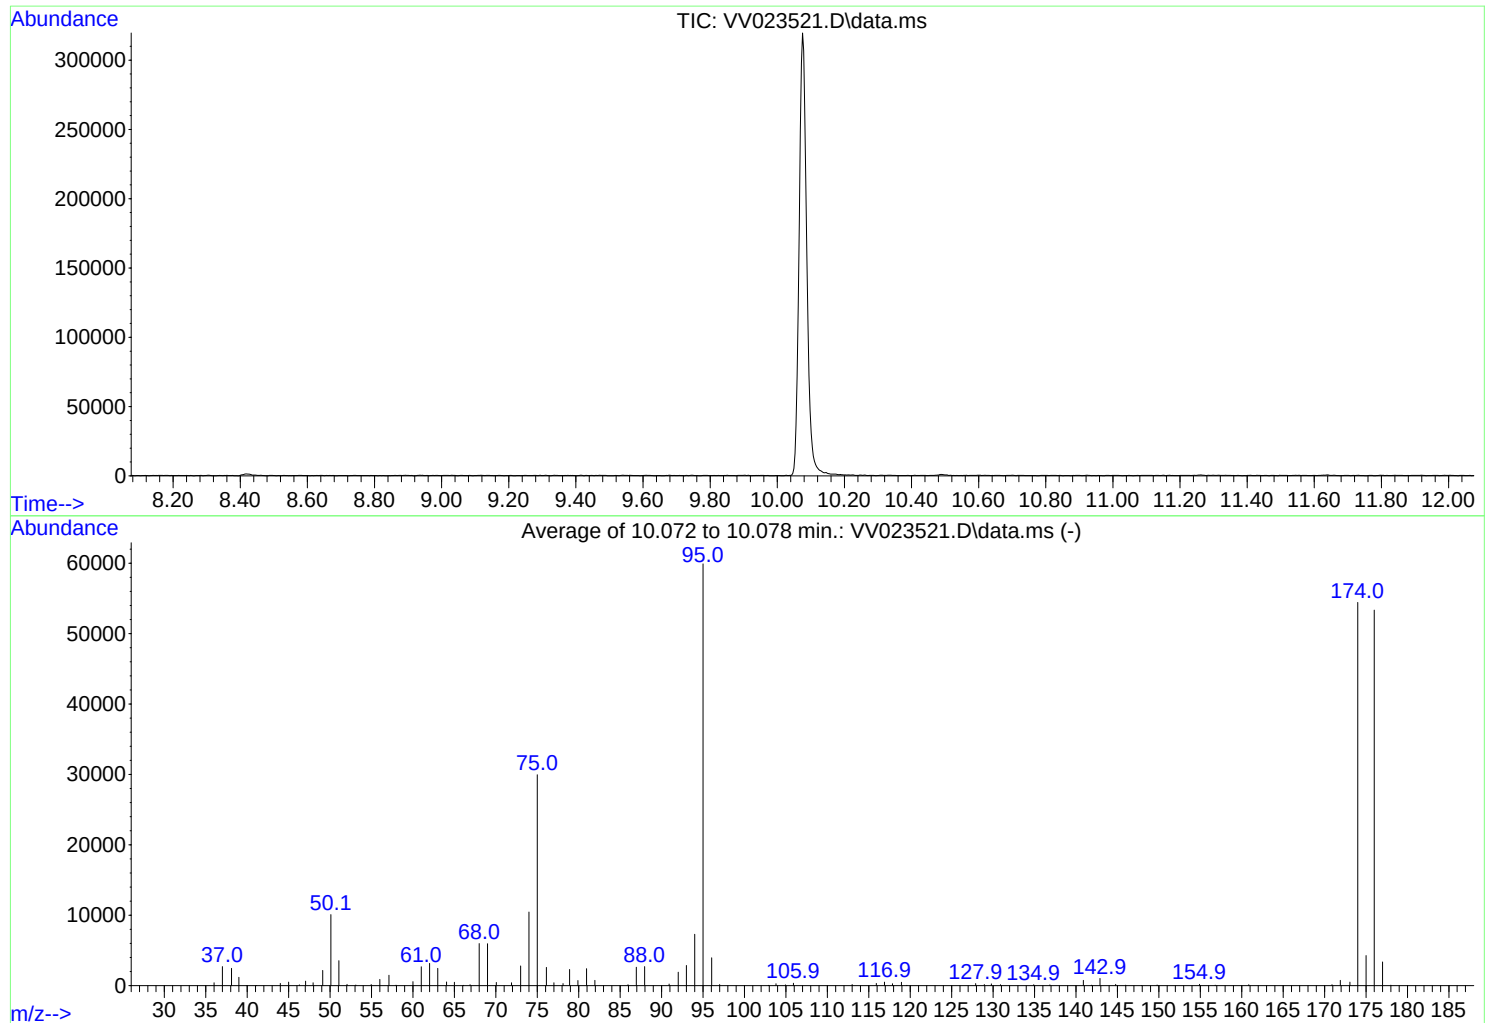

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	10098	PASS
75	95	30	80	50.0	29955	PASS
95	95	100	100	100.0	59912	PASS
96	95	5	9	6.6	3966	PASS
173	174	0.00	2	0.9	495	PASS
174	95	50	120	90.8	54427	PASS
175	174	5	9	7.8	4268	PASS
176	174	95	105	98.0	53352	PASS
177	176	5	10	6.3	3368	PASS

m/z	Abundance
39.90	110.0
44.00	140.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	377.0
37.00	2623.0
38.10	2440.0
39.00	1259.0
40.20	132.0
44.00	478.0
45.00	533.0
46.30	176.0
47.00	786.0
47.90	400.0
49.10	2266.0
50.10	10101.0
51.00	3582.0
52.10	191.0
53.10	139.0
54.90	156.0
56.00	846.0
57.10	1517.0
57.90	103.0
60.00	593.0
61.00	2570.0
62.00	3127.0
63.00	2438.0
64.00	519.0
65.00	467.0
66.10	111.0
66.90	117.0
68.00	5966.0
69.00	5817.0
70.10	474.0
71.90	405.0
73.00	2797.0
74.00	10259.0
75.00	29336.0
76.10	2738.0
77.00	417.0
78.10	249.0
78.90	2150.0
79.90	723.0
80.90	2407.0
81.90	677.0
86.00	134.0
87.00	2529.0
87.90	2896.0
90.90	225.0
92.00	1683.0
93.00	2818.0
94.00	7197.0
95.00	58072.0
96.00	3855.0
97.00	160.0
103.80	270.0
104.90	124.0
105.90	283.0
113.00	132.0
115.90	283.0
116.90	480.0
117.80	284.0
118.90	427.0
127.90	272.0
128.90	135.0
129.80	248.0
130.90	111.0
134.90	109.0
136.80	126.0
140.90	739.0
142.90	998.0
144.80	183.0
146.00	117.0
147.90	102.0
149.80	138.0
154.90	181.0
161.00	113.0
170.90	158.0
171.90	686.0
174.00	51256.0
175.00	4152.0
176.00	50512.0
177.00	3279.0
178.00	127.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	405.0
37.00	2857.0
38.10	2579.0
39.00	1191.0
40.00	129.0
41.10	106.0
44.00	473.0
45.00	519.0
46.30	146.0
47.10	647.0
47.90	407.0
49.10	2220.0
50.10	10357.0
51.00	3726.0
52.10	189.0
53.10	128.0
55.00	149.0
56.00	935.0
57.10	1505.0
60.00	575.0
61.00	2750.0
62.00	3294.0
63.00	2550.0
64.10	549.0
65.00	487.0
66.90	142.0
68.00	6185.0
69.00	6202.0
70.10	457.0
71.90	430.0
73.00	2873.0
74.00	10850.0
75.00	30880.0
76.10	2661.0
77.00	425.0
78.10	317.0
78.90	2379.0
79.90	751.0
81.00	2458.0
81.90	775.0
86.00	134.0
86.90	2689.0
87.90	2761.0
90.90	249.0
92.00	2002.0
93.00	2943.0
94.00	7540.0
95.00	62168.0
96.10	4162.0
97.00	152.0
103.80	294.0
104.90	131.0
105.90	351.0
113.00	165.0
115.90	338.0
116.90	524.0
117.90	288.0
118.90	495.0
119.60	108.0
127.90	314.0
129.00	168.0
129.80	257.0
130.90	136.0
134.90	136.0
136.80	131.0
140.90	818.0
141.90	108.0
142.90	1069.0
144.80	196.0
146.00	119.0
149.80	117.0
154.90	207.0
156.80	100.0
160.80	154.0
170.90	142.0
171.90	755.0
173.10	757.0
174.00	56448.0
175.00	4432.0
176.00	55304.0
177.00	3464.0
178.00	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235

m/z	Abundance
36.00	426.0
37.00	2666.0
38.10	2383.0
39.00	1077.0
40.00	134.0
44.00	426.0
45.00	426.0
47.10	472.0
48.00	394.0
49.10	1992.0
50.10	9837.0
51.10	3360.0
52.00	189.0
55.00	147.0
56.00	903.0
57.10	1410.0
58.00	103.0
60.00	530.0
61.00	2728.0
62.00	3064.0
63.00	2356.0
64.10	480.0
65.00	464.0
66.90	180.0
68.00	5758.0
69.00	5868.0
70.00	469.0
71.90	392.0
73.00	2727.0
74.00	10253.0
75.00	29648.0
76.10	2366.0
77.00	364.0
78.10	325.0
78.90	2382.0
79.90	736.0
80.90	2342.0
82.00	777.0
85.80	134.0
86.90	2641.0
88.00	2449.0
90.90	234.0
92.00	2015.0
93.00	2829.0
94.00	7180.0
95.00	59496.0
96.10	3880.0
97.00	145.0
102.90	107.0
103.80	274.0
105.00	112.0
105.90	363.0
113.00	165.0
115.90	346.0
116.90	497.0
117.90	275.0
119.00	494.0
127.90	297.0
129.00	179.0
129.80	254.0
130.90	146.0
134.90	155.0
136.90	105.0
140.90	711.0
141.90	116.0
142.90	1001.0
144.80	182.0
154.90	188.0
156.80	107.0
160.80	163.0
170.90	123.0
171.90	806.0
173.00	728.0
174.00	55576.0
175.00	4221.0
176.00	54240.0
177.00	3361.0

Instrument :
MSVOA_V
ClientSampleId :
BFB235