

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029006.D
 Acq On : 16 Nov 2022 10:53
 Operator : SY/MD
 Sample : VV1116WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Quant Time: Nov 17 02:51:10 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 17 02:49:50 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	251635	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	234084	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.239	152	108013	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	74577	4.861	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	97.200%
7) Chloroethane-d5	1.565	69	61314	4.546	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.000%
11) 1,1-Dichloroethene-d2	2.102	63	101481	3.630	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	72.600%
20) 2-Butanone-d5	3.899	46	74523	29.020	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	58.040%
24) Chloroform-d	4.339	84	158254	5.025	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	100.400%
26) 1,2-Dichloroethane-d4	5.024	65	71846	5.070	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.400%
32) Benzene-d6	5.040	84	340724	4.876	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.600%
36) 1,2-Dichloropropane-d6	6.063	67	95426	4.891	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.800%
41) Toluene-d8	7.310	98	320026	5.088	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	101.800%
43) trans-1,3-Dichloroprop...	7.619	79	31960	5.022	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	100.400%
46) 2-Hexanone-d5	8.088	63	122497	45.099	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.200%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	62785	4.641	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.800%
66) 1,2-Dichlorobenzene-d4	11.616	152	111146	5.752	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	115.000%
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	10369	0.526	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029006.D
Acq On : 16 Nov 2022 10:53
Operator : SY/MD
Sample : VV1116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Time: Nov 17 02:51:10 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 17 02:49:50 2022
Response via : Initial Calibration

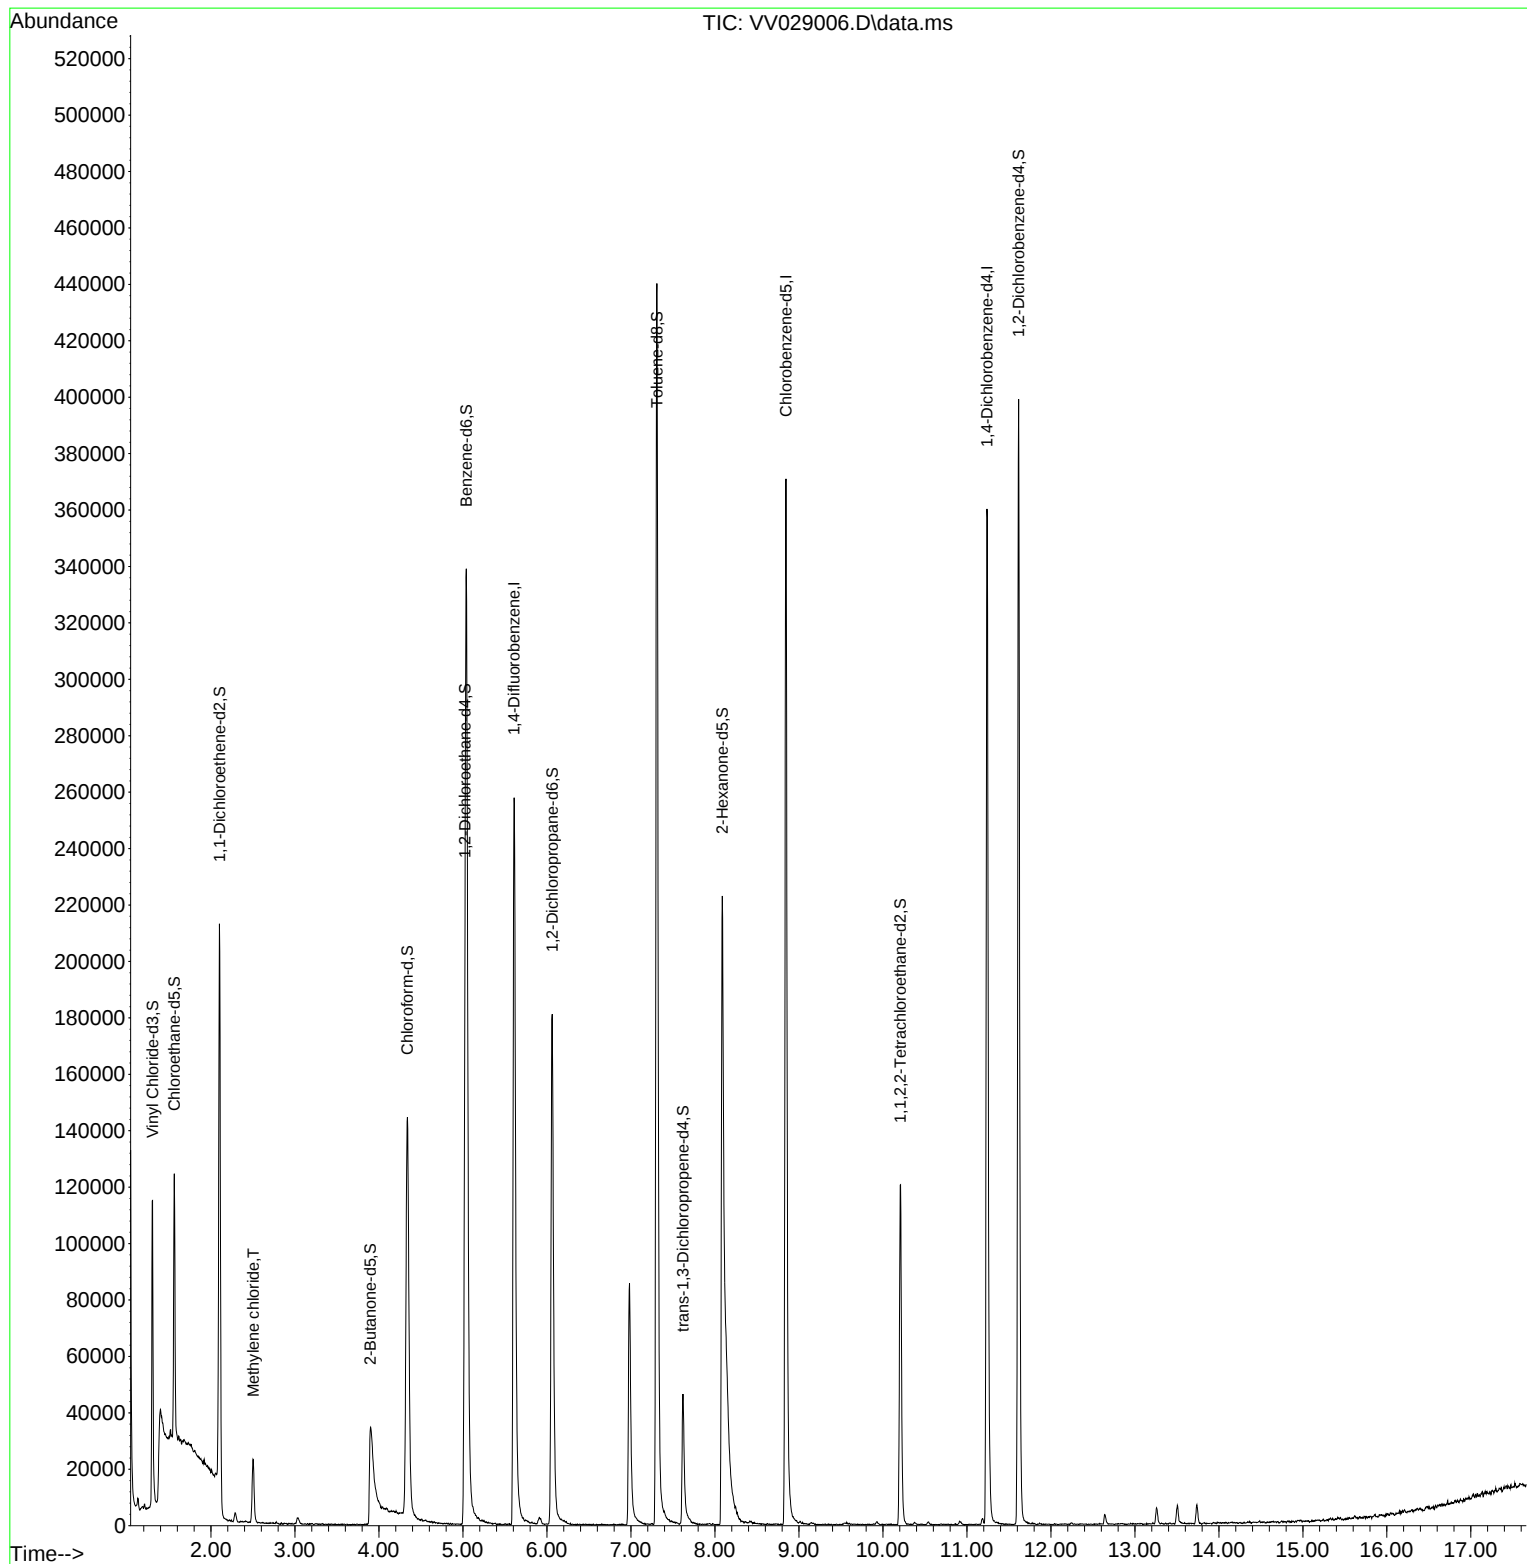

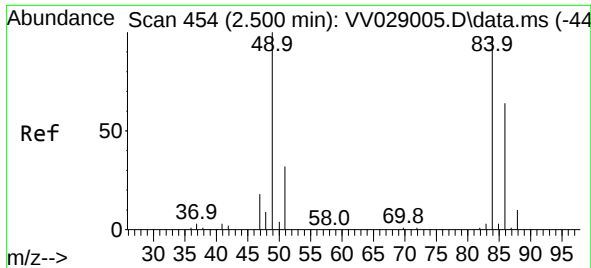

#16

Methylene chloride

Concen: 0.526 ug/L

RT: 2.503 min Scan# 4

Delta R.T. 0.003 min

Lab File: VV029006.D


Acq: 16 Nov 2022 10:53

Instrument :

MSVOA_V

ClientSampleId :

VBLK264

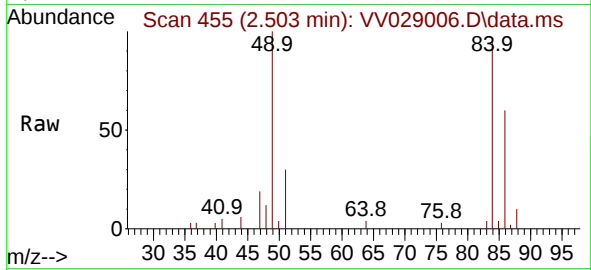

Tgt Ion: 84 Resp: 10369

Ion Ratio Lower Upper

84 100

86 63.3 45.8 85.0

49 105.3 75.5 140.1

