

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029031.D
 Acq On : 16 Nov 2022 21:20
 Operator : SY/MD
 Sample : VV1116WBL02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK265

Quant Time: Nov 17 04:20:40 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 17 04:20:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	267808	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	247239	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	115055	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	77641	4.755	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.200%
7) Chloroethane-d5	1.564	69	62736	4.371	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.400%
11) 1,1-Dichloroethene-d2	2.105	63	103598	3.482	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.600%
20) 2-Butanone-d5	3.905	46	83579	30.581	ug/L	0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	61.160%
24) Chloroform-d	4.346	84	158961	4.742	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.800%
26) 1,2-Dichloroethane-d4	5.027	65	74923	4.968	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	99.400%
32) Benzene-d6	5.043	84	351704	4.766	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	95.400%
36) 1,2-Dichloropropane-d6	6.066	67	99618	4.834	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	96.600%
41) Toluene-d8	7.310	98	324035	4.878	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.600%
43) trans-1,3-Dichloroprop...	7.622	79	32520	4.839	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	96.800%
46) 2-Hexanone-d5	8.088	63	129317	45.077	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.160%
56) 1,1,2,2-Tetrachloroeth...	10.207	84	70533	4.937	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.800%
66) 1,2-Dichlorobenzene-d4	11.615	152	117725	5.719	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	114.400%
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	6084	0.290	ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029031.D
Acq On : 16 Nov 2022 21:20
Operator : SY/MD
Sample : VV1116WBL02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK265


Quant Time: Nov 17 04:20:40 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 17 04:20:13 2022
Response via : Initial Calibration

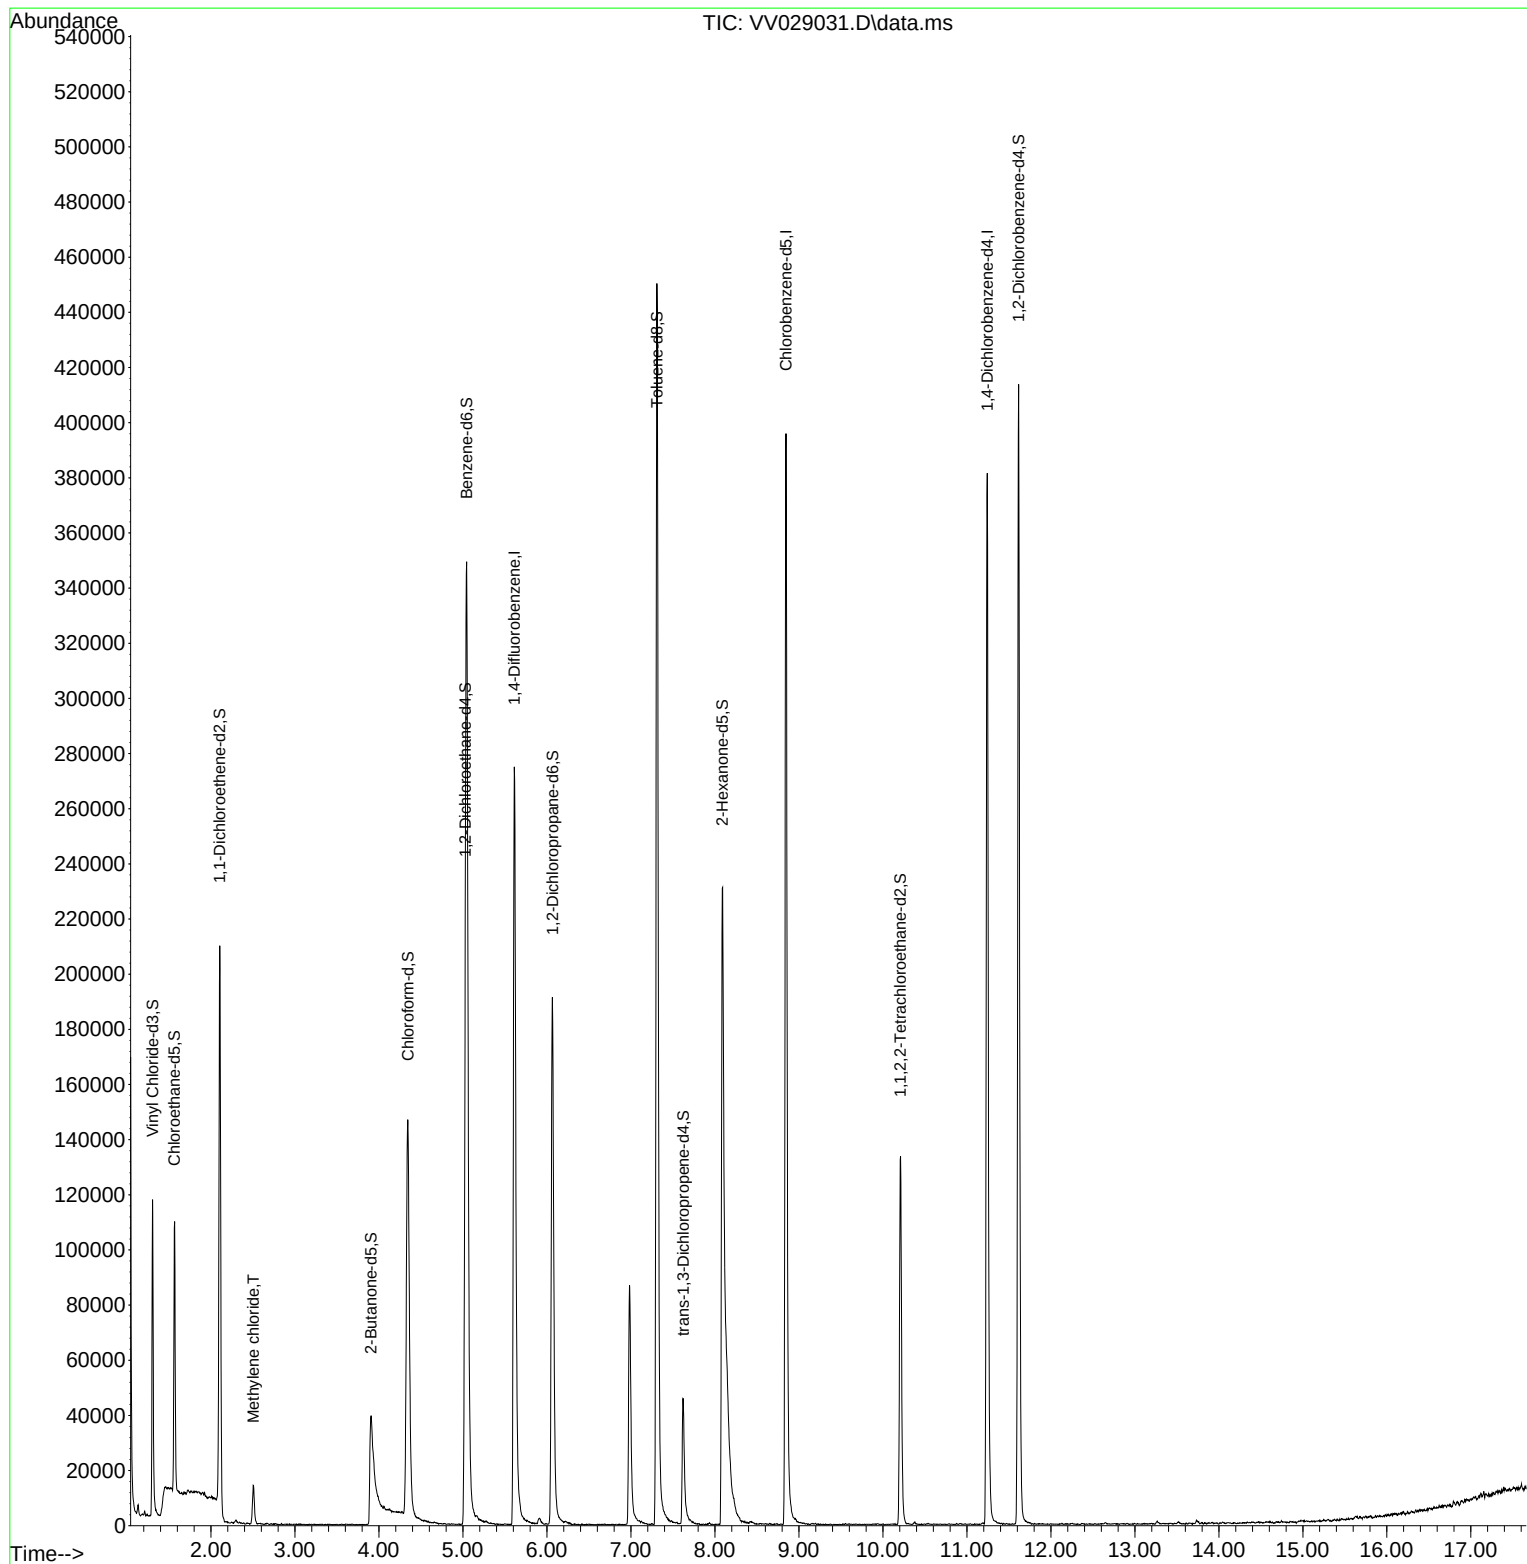

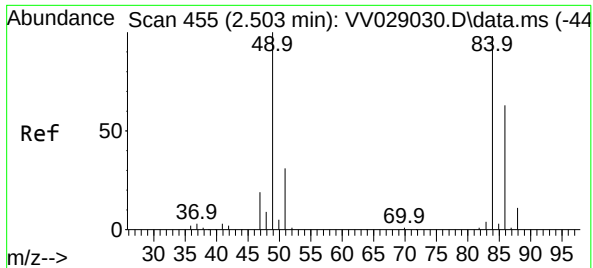

#16
Methylene chloride
Concen: 0.290 ug/L
RT: 2.506 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV029031.D
Acq: 16 Nov 2022 21:20

Instrument :
MSVOA_V
ClientSampleId :
VBLK265

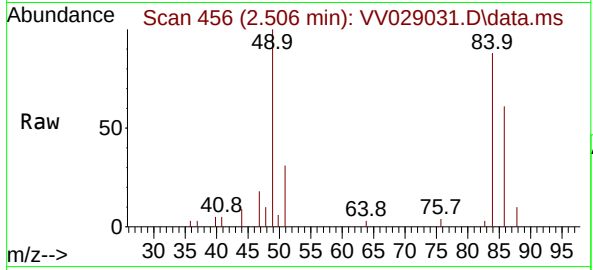

Tgt Ion:	84	Resp:	6084
Ion	Ratio	Lower	Upper
84	100		
86	69.4	45.8	85.0
49	120.9	75.5	140.1

