

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029006.D
 Acq On : 16 Nov 2022 10:53
 Operator : SY/MD
 Sample : VV1116WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029006.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	97	rBV	107531	116680	13.66%	1.735%
2	1.397	100	111	115	rBV2	32363	63196	7.40%	0.940%
3	1.565	156	163	176	rVB	94430	109657	12.84%	1.631%
4	2.102	321	330	353	rVB	211057	315764	36.98%	4.697%
5	2.500	444	454	468	rBV	22350	36963	4.33%	0.550%
6	3.902	880	890	918	rBV2	34238	131356	15.38%	1.954%
7	4.339	1010	1026	1052	rVB	141160	351420	41.15%	5.227%
8	5.040	1228	1244	1279	rBV2	338593	853911	100.00%	12.701%
9	5.609	1409	1421	1452	rBV	257699	544820	63.80%	8.104%
10	6.063	1545	1562	1593	rBV	180801	382951	44.85%	5.696%
11	6.982	1835	1848	1879	rBV2	85624	171899	20.13%	2.557%
12	7.310	1938	1950	1975	rBV	439926	791273	92.66%	11.769%
13	7.619	2032	2046	2078	rBV	46180	91750	10.74%	1.365%
14	8.088	2181	2192	2239	rBV	222846	653918	76.58%	9.726%
15	8.847	2416	2428	2452	rBV	370695	636900	74.59%	9.473%
16	10.211	2840	2852	2874	rBV	120432	205960	24.12%	3.063%
17	11.239	3162	3172	3197	rBV	359594	595699	69.76%	8.860%
18	11.616	3276	3289	3316	rBV	398704	637778	74.69%	9.486%
19	13.259	3791	3800	3814	rVB3	5746	9315	1.09%	0.139%
20	13.506	3866	3877	3886	rBV3	6683	11349	1.33%	0.169%
21	13.738	3941	3949	3959	rBV4	6737	10637	1.25%	0.158%




Sum of corrected areas: 6723196

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029006.D
Acq On : 16 Nov 2022 10:53
Operator : SY/MD
Sample : VV1116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

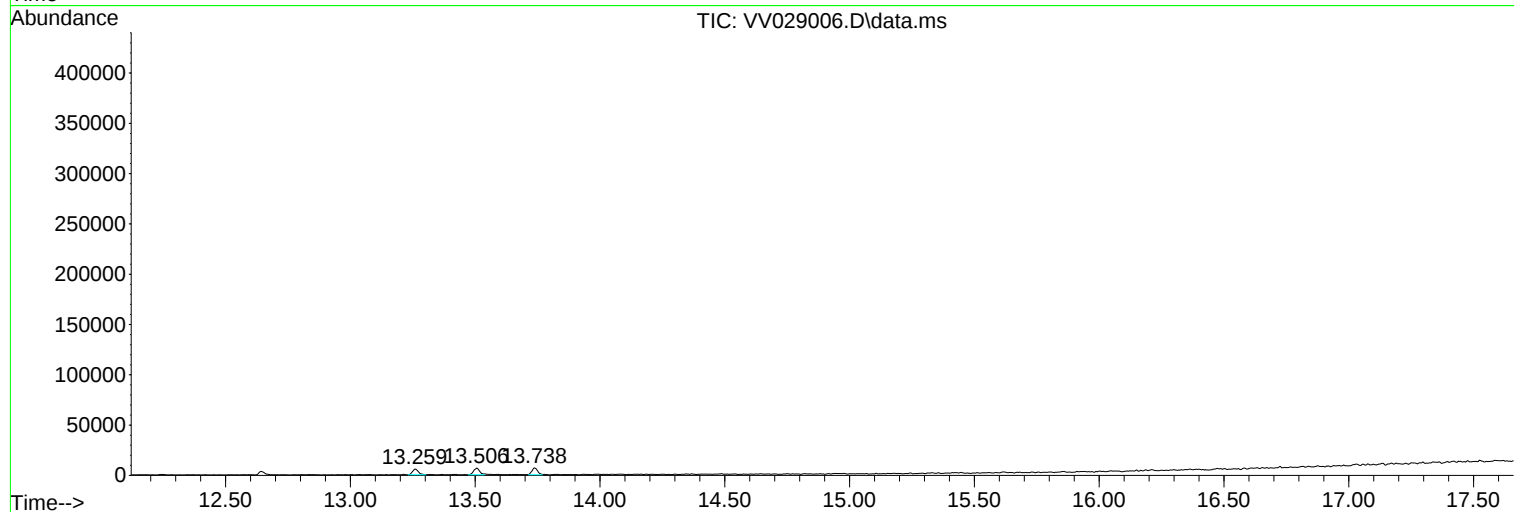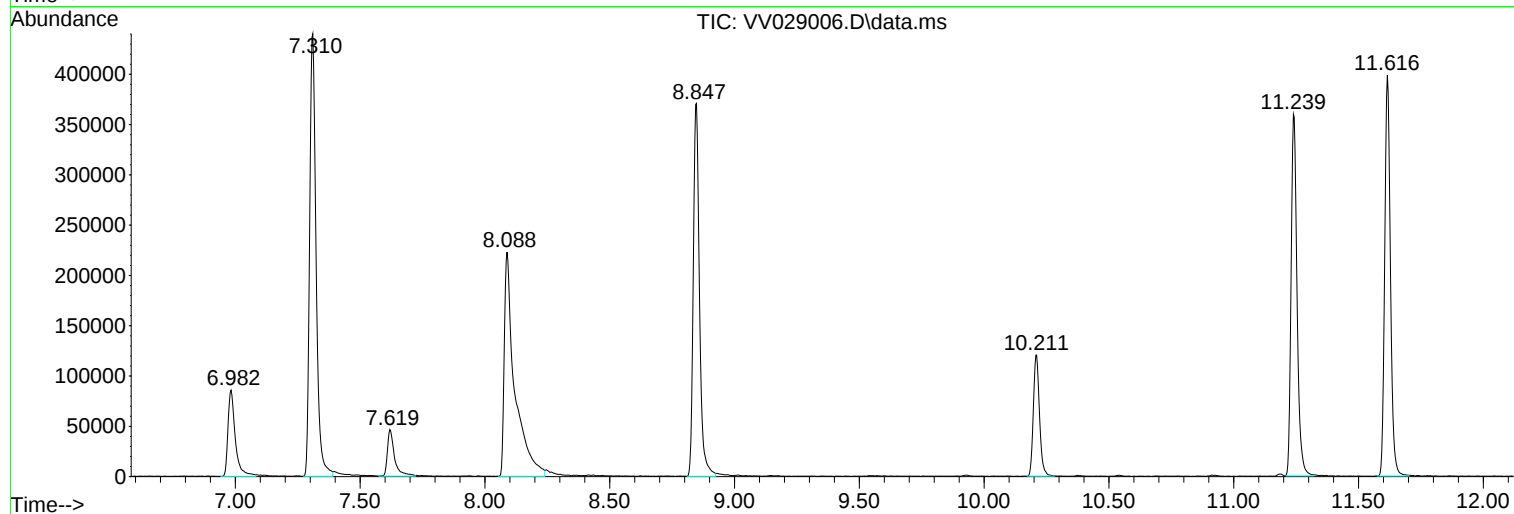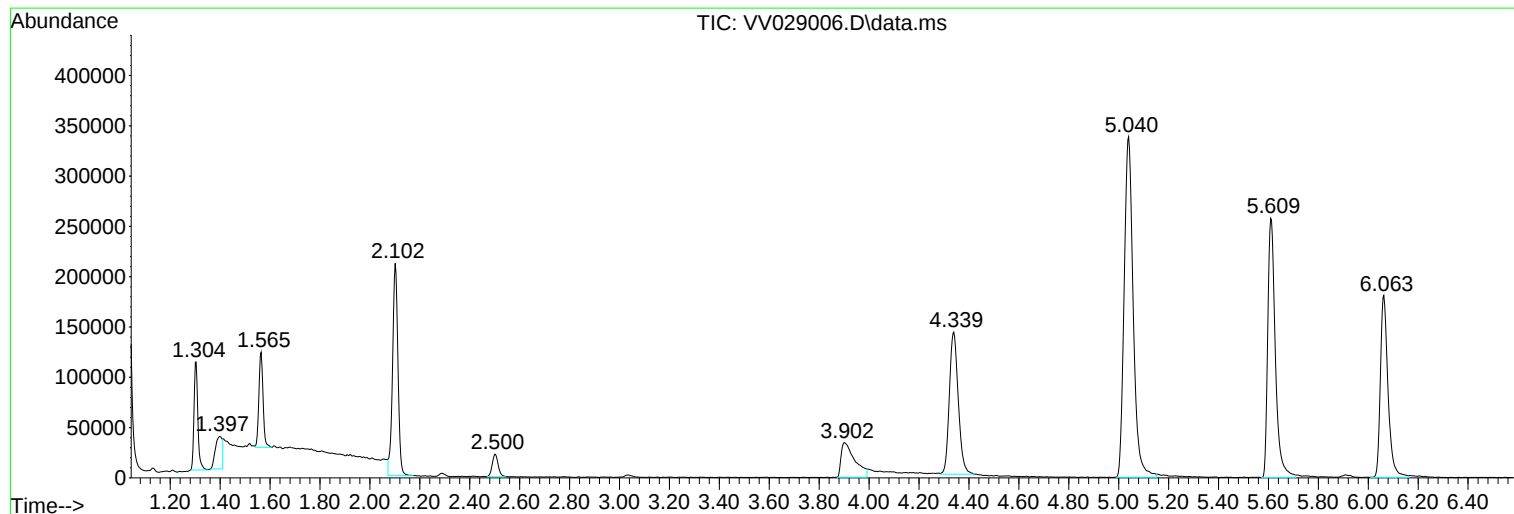

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029006.D
Acq On : 16 Nov 2022 10:53
Operator : SY/MD
Sample : VV1116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.397	0.58 ug/L	63196	1,4-Difluorobenzene	5.609

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
3			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
4			Sulfur dioxide	64	O2S	007446-09-5	4
5			Sulfur dioxide	64	O2S	007446-09-5	4

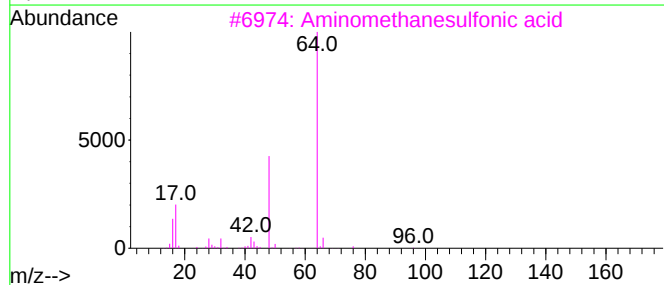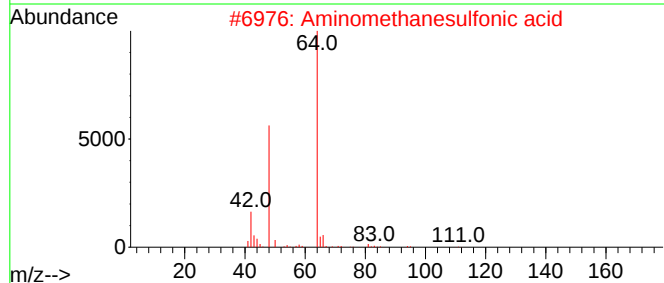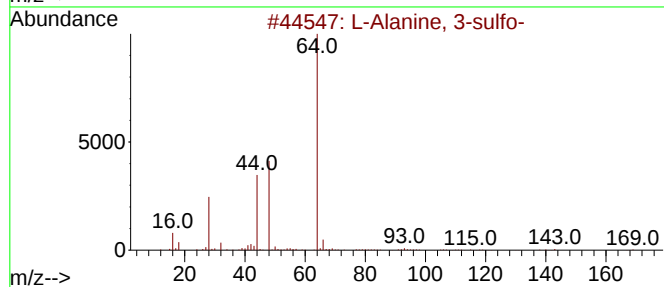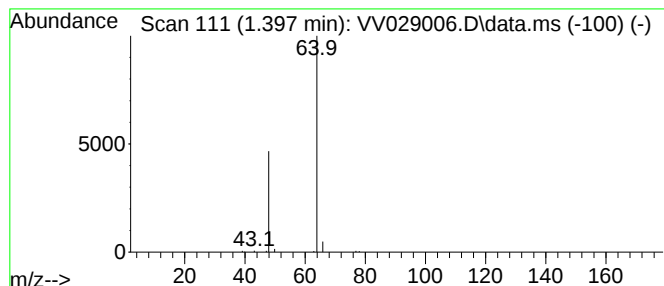

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029006.D
Acq On : 16 Nov 2022 10:53
Operator : SY/MD
Sample : VV1116WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.397	0.6	ug/L	63196	1	5.609	544820	5.0