

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029011.D
 Acq On : 16 Nov 2022 12:52
 Operator : SY/MD
 Sample : N5620-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGC99

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029011.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.182	36	44	48	rBV2	7042	11762	1.62%	0.197%
2	1.237	56	61	69	rVB	8270	9384	1.29%	0.157%
3	1.304	75	82	96	rVB	56156	62218	8.57%	1.043%
4	1.574	158	166	180	rVB	69884	80168	11.05%	1.344%
5	1.986	283	294	301	rBV2	21733	51803	7.14%	0.869%
6	2.111	324	333	362	rVB	133754	219590	30.25%	3.682%
7	3.970	886	911	942	rBV2	49167	220733	30.41%	3.701%
8	4.349	1012	1029	1050	rBV	118737	283781	39.10%	4.759%
9	5.040	1225	1244	1264	rBV2	268740	586992	80.87%	9.843%
10	5.609	1407	1421	1440	rBV	279814	547893	75.49%	9.188%
11	6.069	1546	1564	1584	rBV	171543	350586	48.30%	5.879%
12	6.207	1600	1607	1621	rBV3	3986	9242	1.27%	0.155%
13	6.834	1796	1802	1822	rBV	26080	47878	6.60%	0.803%
14	6.992	1838	1851	1869	rBV	67323	121678	16.76%	2.040%
15	7.320	1941	1953	1973	rBV	330186	565575	77.92%	9.484%
16	7.632	2040	2050	2063	rBV2	36449	62844	8.66%	1.054%
17	8.114	2189	2200	2241	rBV	349134	725822	100.00%	12.171%
18	8.854	2418	2430	2451	rBV	401859	657890	90.64%	11.032%
19	10.214	2838	2853	2871	rBV	138316	214263	29.52%	3.593%
20	10.378	2894	2904	2911	rBV2	5979	9191	1.27%	0.154%
21	11.243	3162	3173	3195	rBV	398614	615658	84.82%	10.324%
22	11.616	3277	3289	3309	rBV	317000	508411	70.05%	8.526%




Sum of corrected areas: 5963362

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029011.D
Acq On : 16 Nov 2022 12:52
Operator : SY/MD
Sample : N5620-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

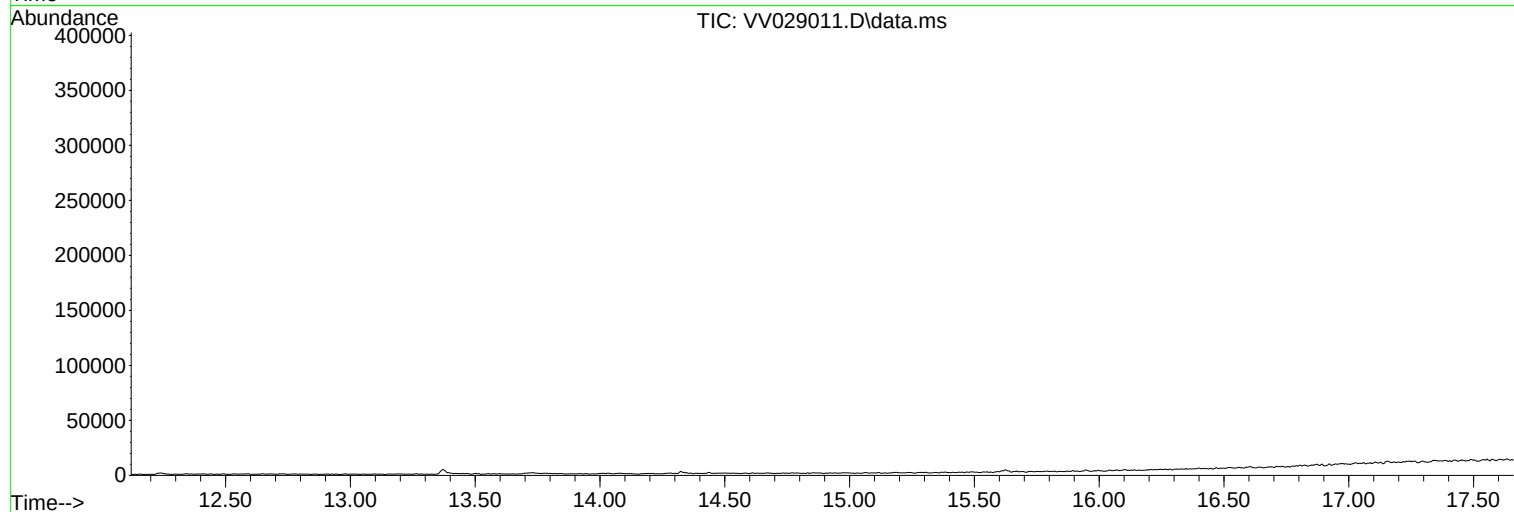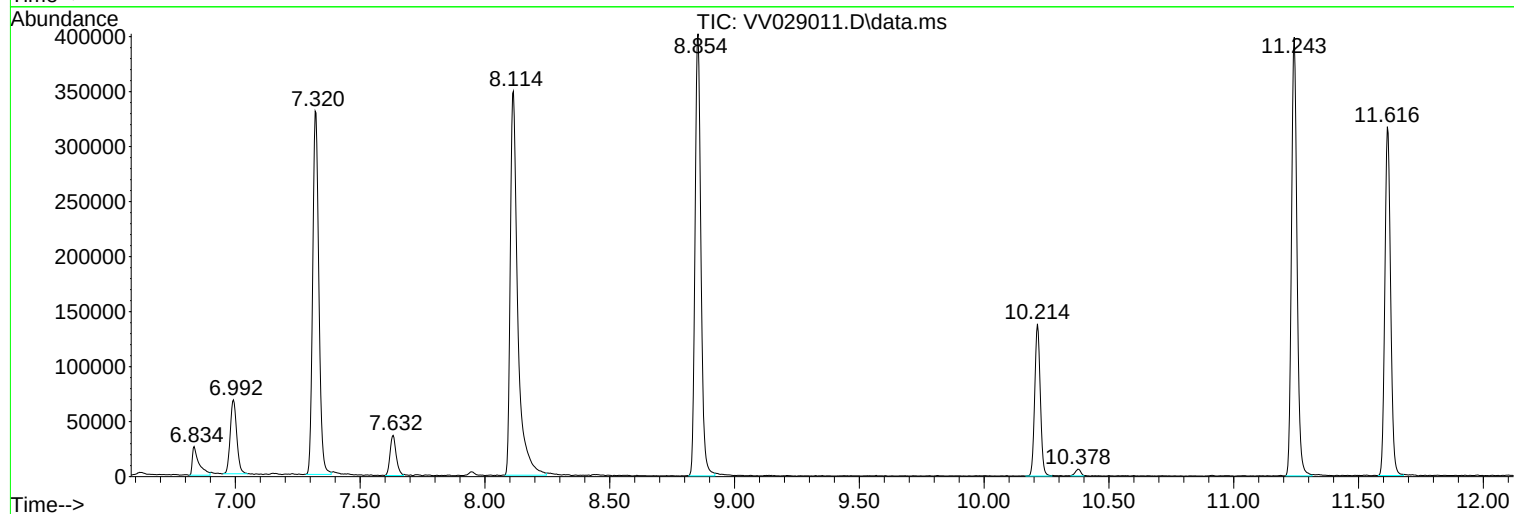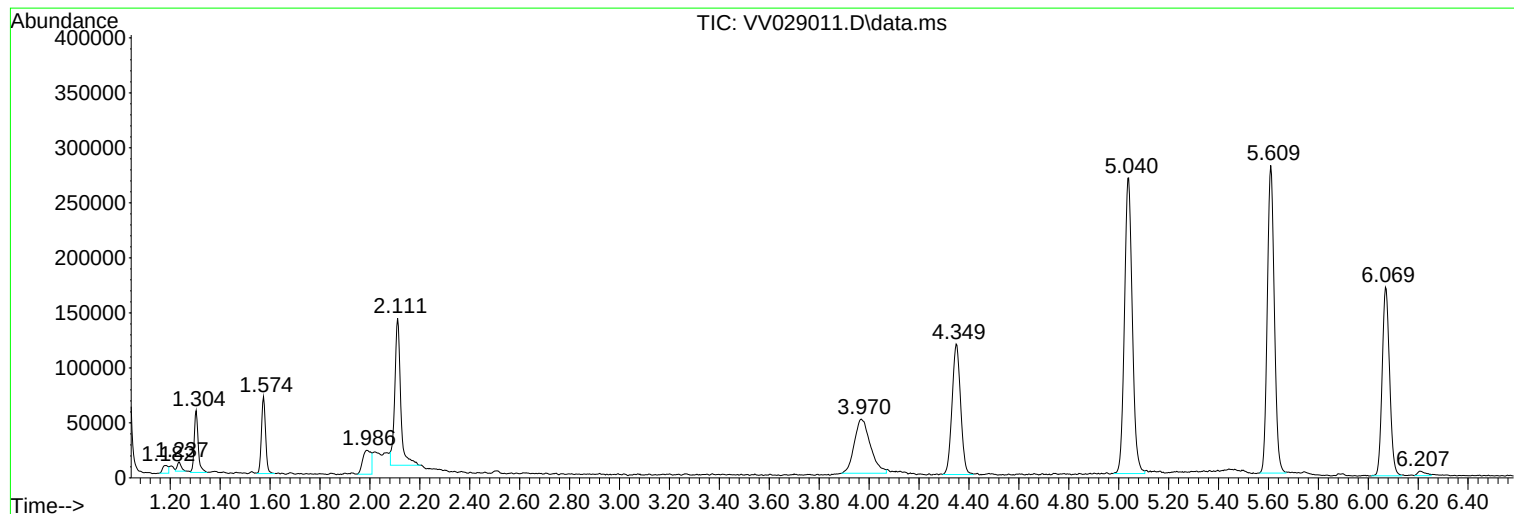

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029011.D
Acq On : 16 Nov 2022 12:52
Operator : SY/MD
Sample : N5620-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029011.D
Acq On : 16 Nov 2022 12:52
Operator : SY/MD
Sample : N5620-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGC99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc