

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029015.D
 Acq On : 16 Nov 2022 14:30
 Operator : SY/MD
 Sample : N5620-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCA3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029015.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	19	25	38	rVB	55677	58532	7.86%	0.961%
2	1.307	76	83	94	rBV	58986	63316	8.50%	1.040%
3	1.439	109	124	126	rBV2	18921	35403	4.76%	0.581%
4	1.568	157	164	180	rVB	78454	90045	12.09%	1.479%
5	2.108	322	332	356	rVB	121982	208871	28.05%	3.430%
6	3.899	880	889	922	rBV2	41017	166773	22.40%	2.739%
7	4.342	1012	1027	1057	rVB2	126721	335334	45.04%	5.507%
8	5.043	1229	1245	1273	rBV2	272042	695700	93.44%	11.424%
9	5.613	1409	1422	1450	rBV	270135	562589	75.57%	9.238%
10	6.066	1550	1563	1594	rBV2	158937	340035	45.67%	5.584%
11	6.985	1838	1849	1870	rBV2	58688	113437	15.24%	1.863%
12	7.313	1939	1951	1977	rBV	299110	550307	73.92%	9.037%
13	7.622	2038	2047	2067	rBV2	30235	60698	8.15%	0.997%
14	8.092	2182	2193	2238	rBV2	241028	744506	100.00%	12.226%
15	8.847	2417	2428	2471	rBV	388115	671185	90.15%	11.022%
16	10.210	2837	2852	2875	rBV	132327	225518	30.29%	3.703%
17	11.243	3161	3173	3196	rBV	392881	632662	84.98%	10.389%
18	11.535	3256	3264	3278	rBV5	5982	12849	1.73%	0.211%
19	11.616	3278	3289	3312	rVB	314271	521873	70.10%	8.570%




Sum of corrected areas: 6089633

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029015.D
Acq On : 16 Nov 2022 14:30
Operator : SY/MD
Sample : N5620-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

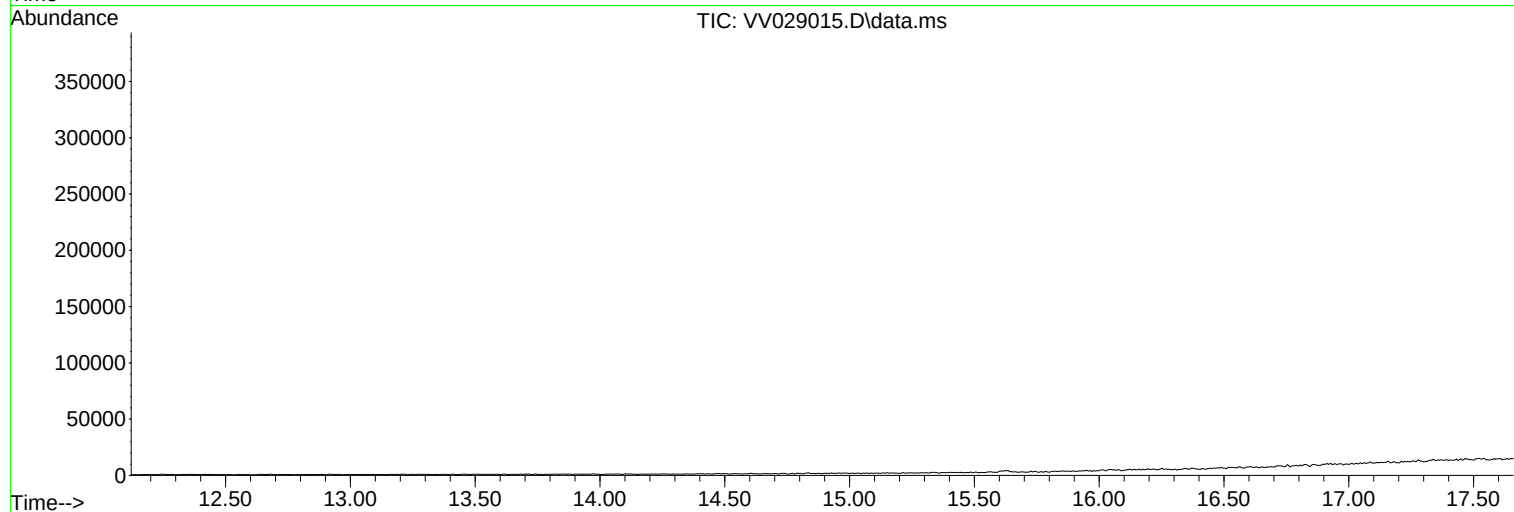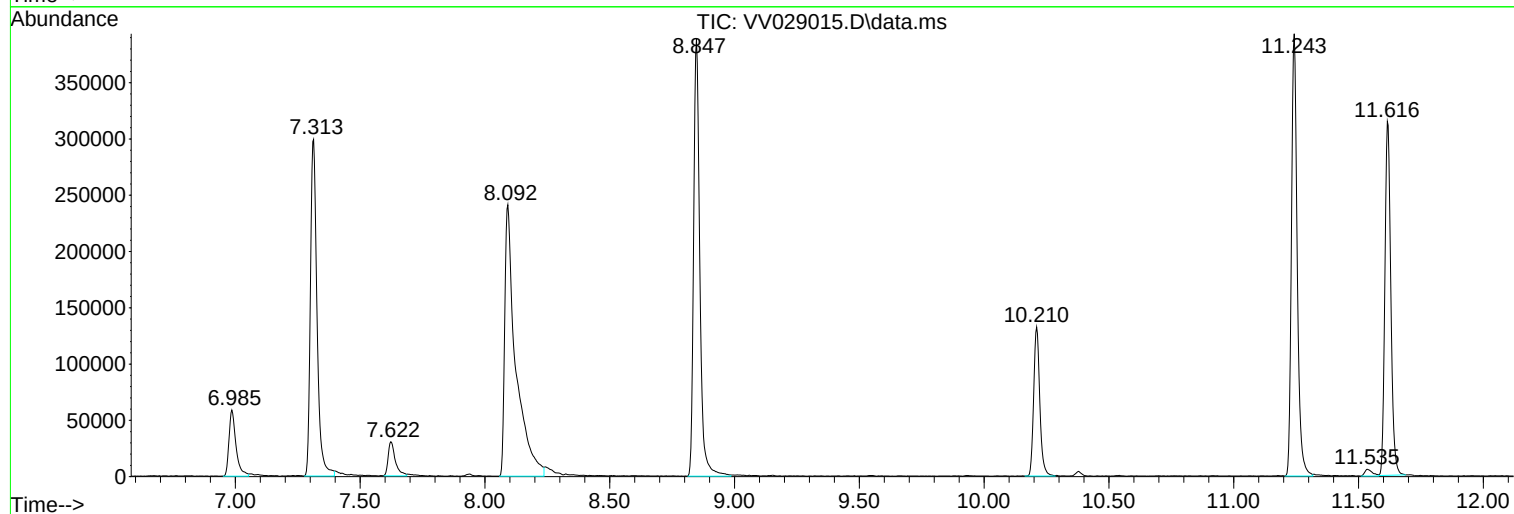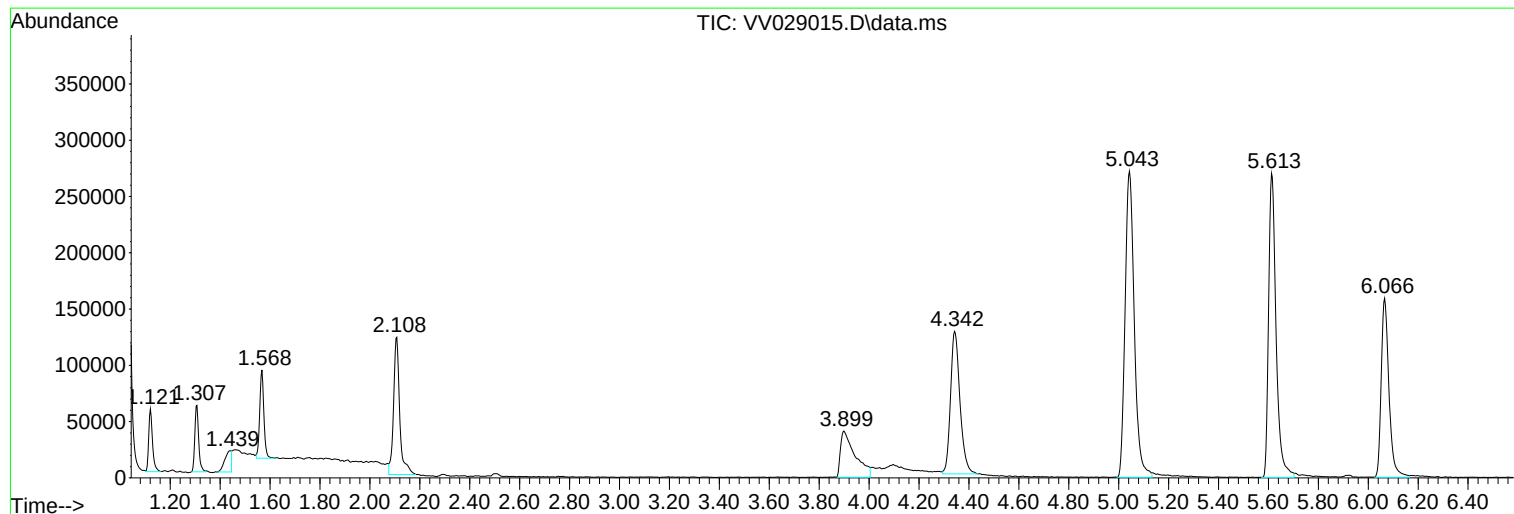

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029015.D
Acq On : 16 Nov 2022 14:30
Operator : SY/MD
Sample : N5620-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCA3








Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.121	0.52 ug/L	58532	1,4-Difluorobenzene	5.613

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Carbonyl sulfide	60	COS	000463-58-1	5
2			Carbonyl sulfide	60	COS	000463-58-1	5
3			Thiirane	60	C2H4S	000420-12-2	4
4			Thiirane	60	C2H4S	000420-12-2	4
5			Thiirane	60	C2H4S	000420-12-2	4

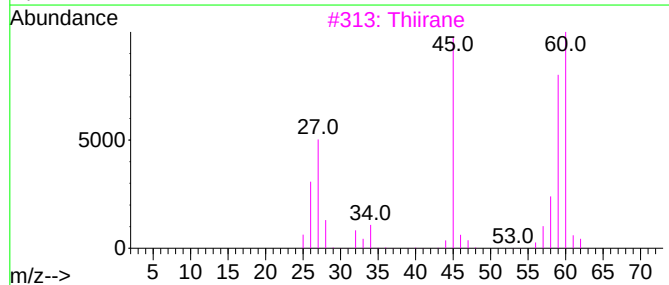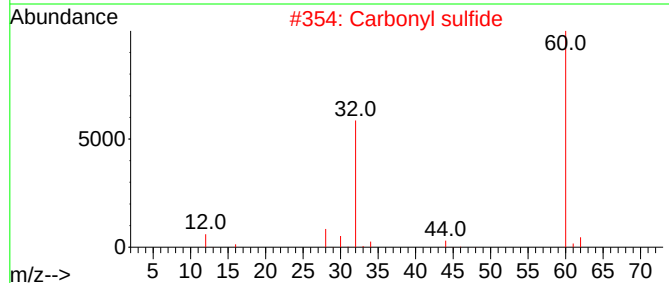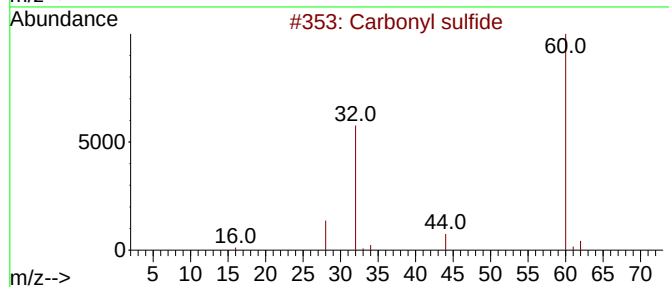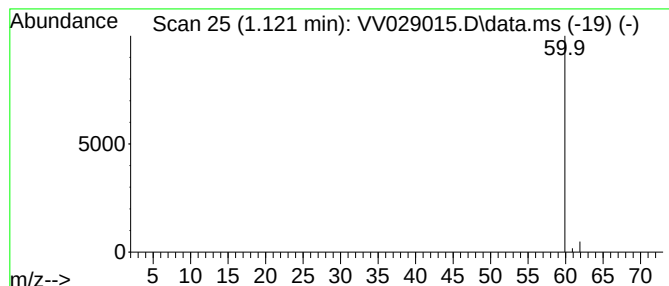

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029015.D
Acq On : 16 Nov 2022 14:30
Operator : SY/MD
Sample : N5620-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.121	0.5	ug/L	58532	1	5.613	562589	5.0