

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029022.D
 Acq On : 16 Nov 2022 17:15
 Operator : SY/MD
 Sample : N5620-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029022.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	96	rVB	64243	69631	8.96%	1.124%
2	1.410	104	115	117	rBV2	28562	44056	5.67%	0.711%
3	1.568	157	164	178	rVB	79009	90618	11.66%	1.463%
4	2.105	322	331	345	rVB	134203	204791	26.34%	3.306%
5	3.896	876	888	922	rBV2	43875	181748	23.38%	2.934%
6	4.098	941	951	965	rVB5	6735	16059	2.07%	0.259%
7	4.343	1012	1027	1063	rVB	129524	345227	44.41%	5.574%
8	5.043	1230	1245	1280	rBV2	282044	729269	93.80%	11.775%
9	5.613	1410	1422	1452	rBV	264410	557598	71.72%	9.003%
10	5.921	1509	1518	1533	rVB10	3874	8885	1.14%	0.143%
11	6.066	1550	1563	1593	rBV	168023	356997	45.92%	5.764%
12	6.986	1835	1849	1875	rBV	59446	122633	15.77%	1.980%
13	7.310	1939	1950	1972	rBV	313302	574956	73.96%	9.283%
14	7.622	2038	2047	2065	rBV	32753	62101	7.99%	1.003%
15	7.937	2132	2145	2155	rBV2	7930	14696	1.89%	0.237%
16	8.088	2181	2192	2248	rBV2	245835	777440	100.00%	12.552%
17	8.847	2416	2428	2457	rBV	382033	659220	84.79%	10.644%
18	10.210	2837	2852	2871	rBV	137966	233606	30.05%	3.772%
19	10.378	2891	2904	2917	rBV2	20575	35563	4.57%	0.574%
20	11.243	3162	3173	3194	rBV	350304	585874	75.36%	9.459%
21	11.616	3275	3289	3317	rBV	313747	522662	67.23%	8.439%




Sum of corrected areas: 6193630

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029022.D
Acq On : 16 Nov 2022 17:15
Operator : SY/MD
Sample : N5620-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

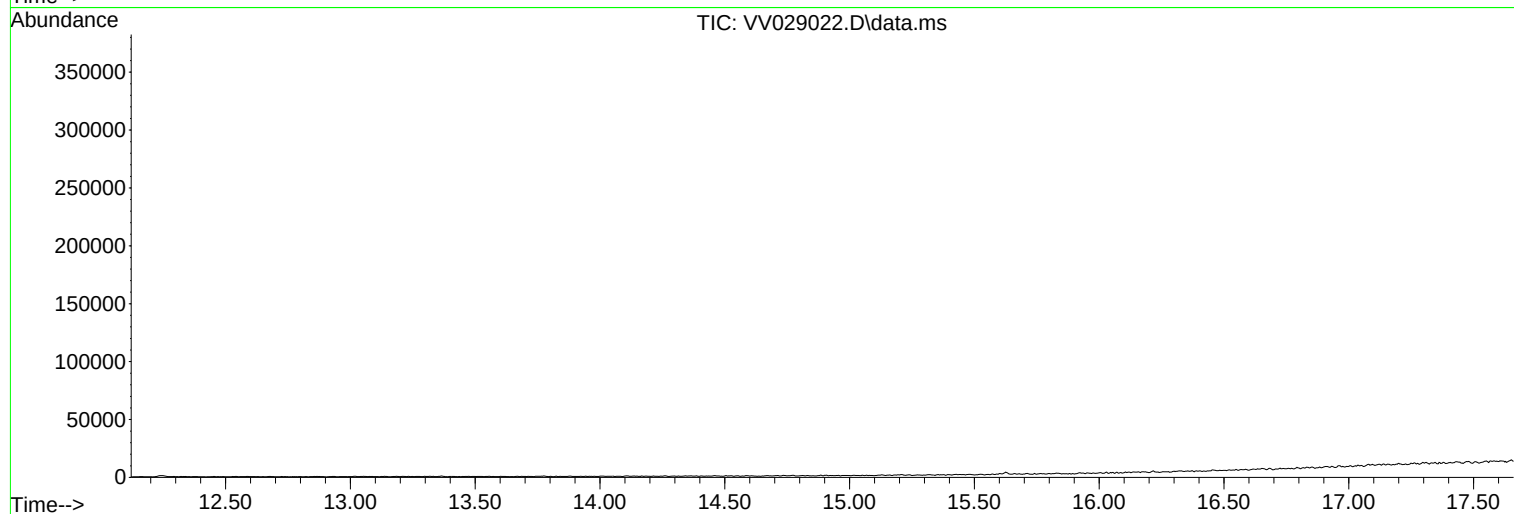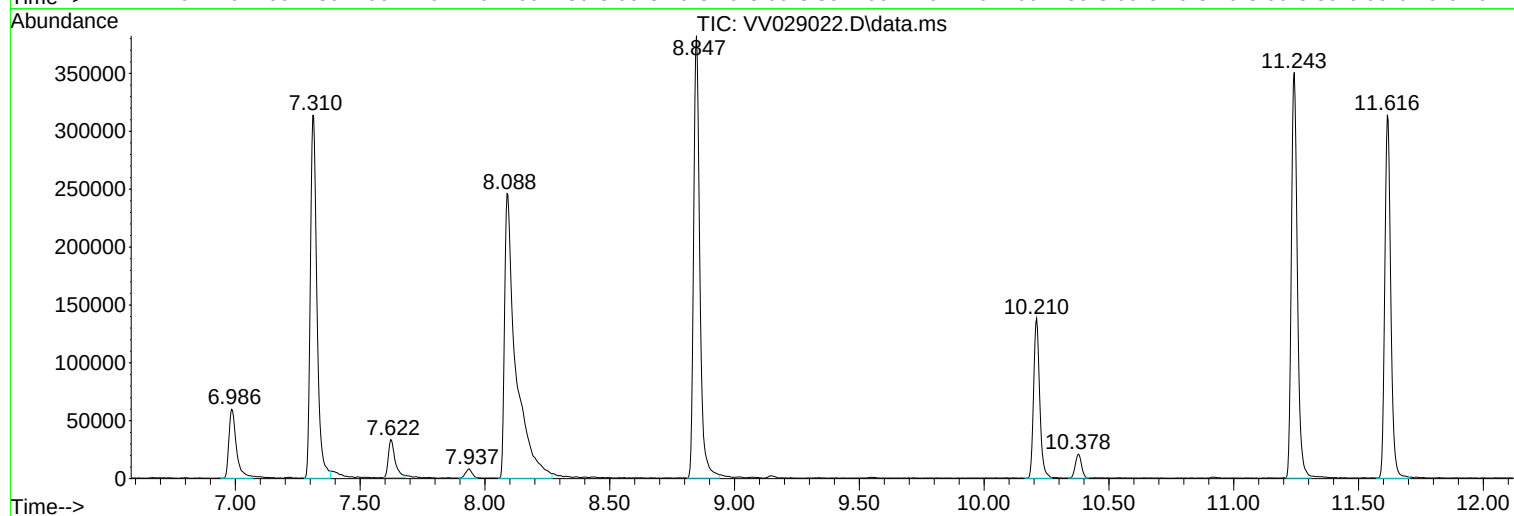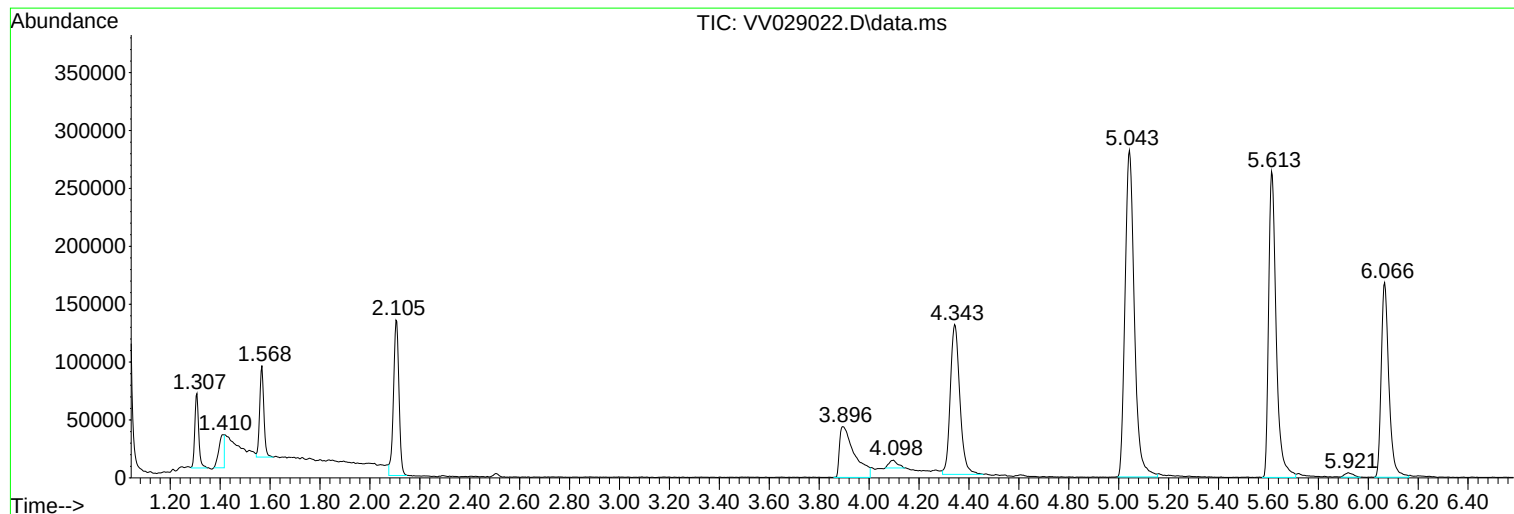

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029022.D
Acq On : 16 Nov 2022 17:15
Operator : SY/MD
Sample : N5620-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029022.D
Acq On : 16 Nov 2022 17:15
Operator : SY/MD
Sample : N5620-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc