

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029026.D
 Acq On : 16 Nov 2022 18:53
 Operator : SY/MD
 Sample : N5620-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCB4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029026.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	94	rBV	61212	64595	8.37%	1.039%
2	1.423	105	119	120	rBV	29074	48349	6.26%	0.778%
3	1.564	157	163	175	rVB	73189	86047	11.15%	1.385%
4	2.105	321	331	351	rVB	138218	212630	27.55%	3.421%
5	3.905	881	891	921	rBV2	44432	175258	22.71%	2.820%
6	4.092	941	949	980	rVB4	10902	35949	4.66%	0.578%
7	4.342	1010	1027	1062	rVB	127949	335319	43.44%	5.395%
8	5.043	1229	1245	1281	rBV2	279927	715678	92.72%	11.516%
9	5.612	1411	1422	1453	rBV	278029	580360	75.19%	9.338%
10	6.066	1548	1563	1590	rBV	165980	348247	45.12%	5.604%
11	6.985	1839	1849	1869	rBV	60748	117277	15.19%	1.887%
12	7.313	1939	1951	1971	rBV	311800	562236	72.84%	9.047%
13	7.622	2038	2047	2072	rBV3	31642	64127	8.31%	1.032%
14	7.931	2133	2143	2161	rVB	6272	11690	1.51%	0.188%
15	8.088	2182	2192	2249	rBV2	275960	771841	100.00%	12.419%
16	8.847	2415	2428	2459	rBV	406045	680018	88.10%	10.942%
17	10.210	2840	2852	2872	rBV	136935	226104	29.29%	3.638%
18	10.374	2892	2903	2917	rBV2	15371	27080	3.51%	0.436%
19	11.242	3162	3173	3195	rBV	395215	635049	82.28%	10.218%
20	11.615	3277	3289	3311	rBV	321014	516940	66.97%	8.318%




Sum of corrected areas: 6214794

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029026.D
Acq On : 16 Nov 2022 18:53
Operator : SY/MD
Sample : N5620-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

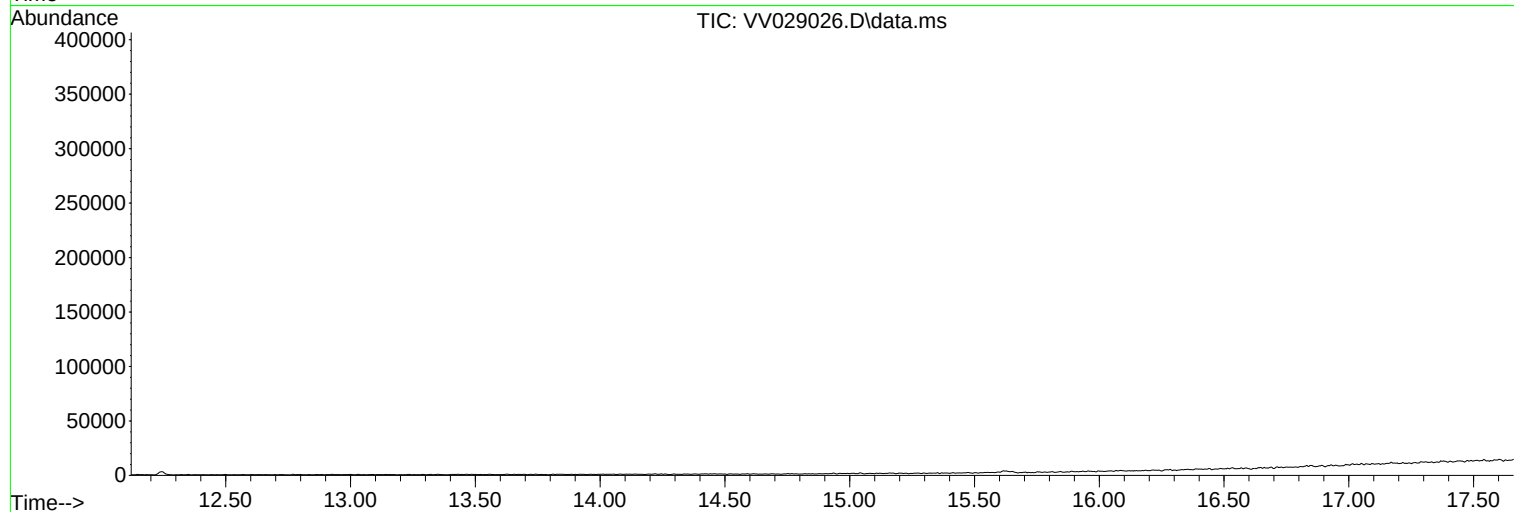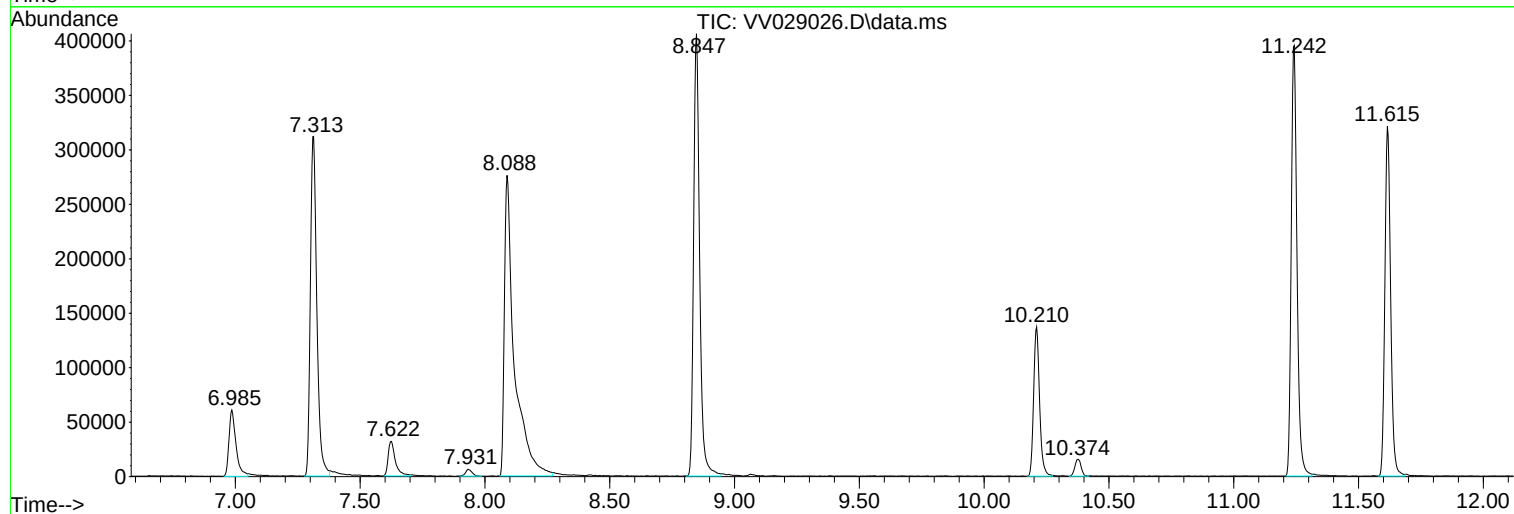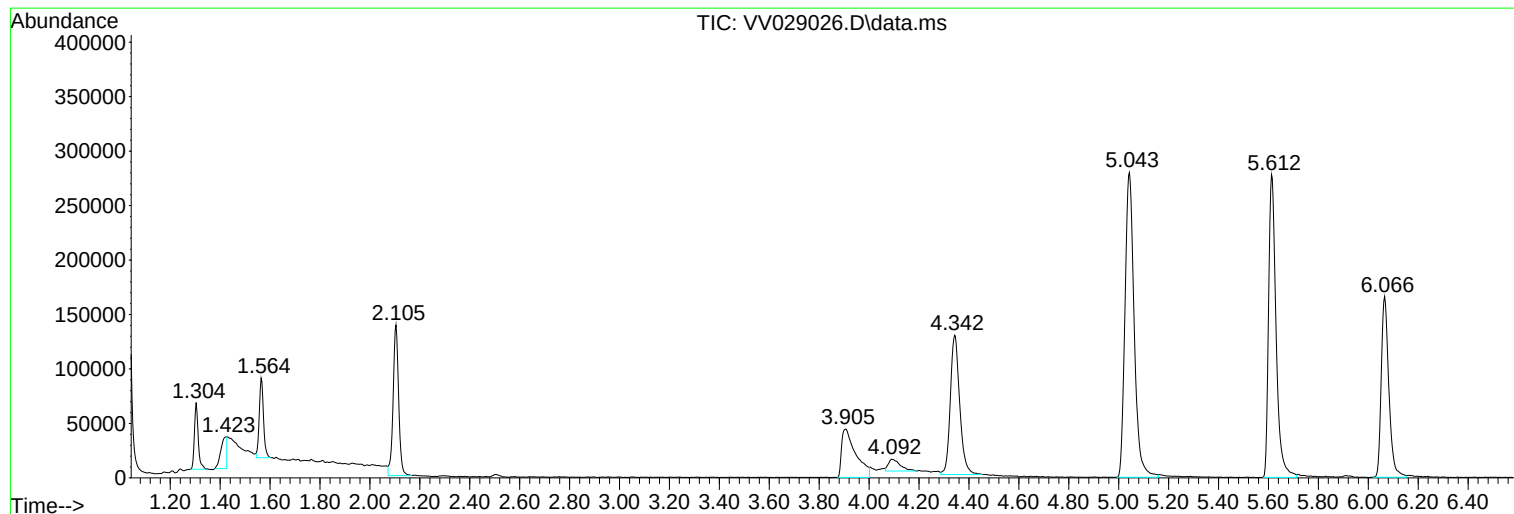

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029026.D
Acq On : 16 Nov 2022 18:53
Operator : SY/MD
Sample : N5620-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029026.D
Acq On : 16 Nov 2022 18:53
Operator : SY/MD
Sample : N5620-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc