

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029028.D
 Acq On : 16 Nov 2022 19:42
 Operator : SY/MD
 Sample : N5620-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCB6

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029028.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	100	rVB	59734	66138	9.02%	1.088%
2	1.410	101	115	116	rBV	34507	55779	7.61%	0.918%
3	1.568	157	164	174	rVB	73693	83764	11.42%	1.378%
4	2.105	322	331	350	rVB	132304	204984	27.95%	3.373%
5	3.899	880	889	928	rBV	42992	176779	24.11%	2.909%
6	4.342	1012	1027	1060	rVB	124359	326623	44.54%	5.375%
7	5.043	1230	1245	1272	rBV3	268421	685899	93.53%	11.287%
8	5.613	1411	1422	1464	rBV	279399	585697	79.87%	9.638%
9	6.066	1549	1563	1594	rBV	159581	338859	46.21%	5.576%
10	6.985	1837	1849	1879	rBV	57018	116191	15.84%	1.912%
11	7.313	1937	1951	1974	rBV	302529	547023	74.60%	9.002%
12	7.622	2039	2047	2076	rBV2	30824	61125	8.34%	1.006%
13	7.937	2133	2145	2158	rVB2	6270	10939	1.49%	0.180%
14	8.092	2183	2193	2255	rBV2	231718	733316	100.00%	12.067%
15	8.847	2416	2428	2459	rBV	399526	685217	93.44%	11.276%
16	10.210	2840	2852	2871	rBV	134246	225864	30.80%	3.717%
17	10.378	2894	2904	2917	rVB2	14545	23815	3.25%	0.392%
18	11.243	3162	3173	3192	rBV	392548	643640	87.77%	10.592%
19	11.616	3277	3289	3313	rBV	304556	505141	68.88%	8.313%




Sum of corrected areas: 6076793

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029028.D
Acq On : 16 Nov 2022 19:42
Operator : SY/MD
Sample : N5620-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

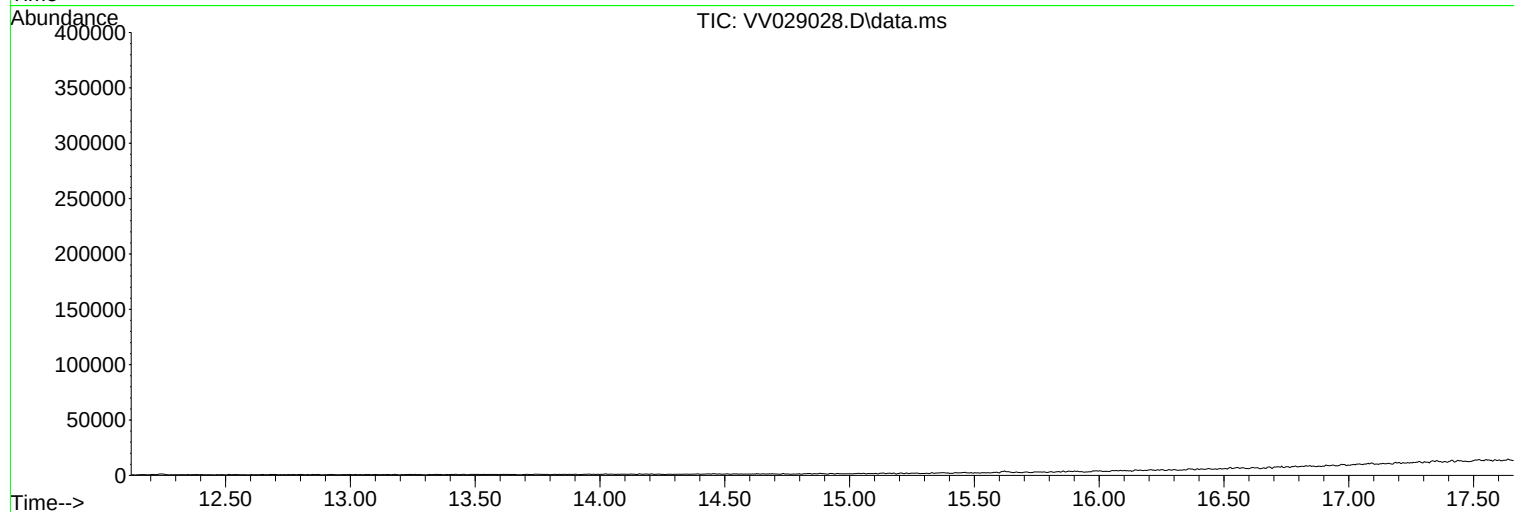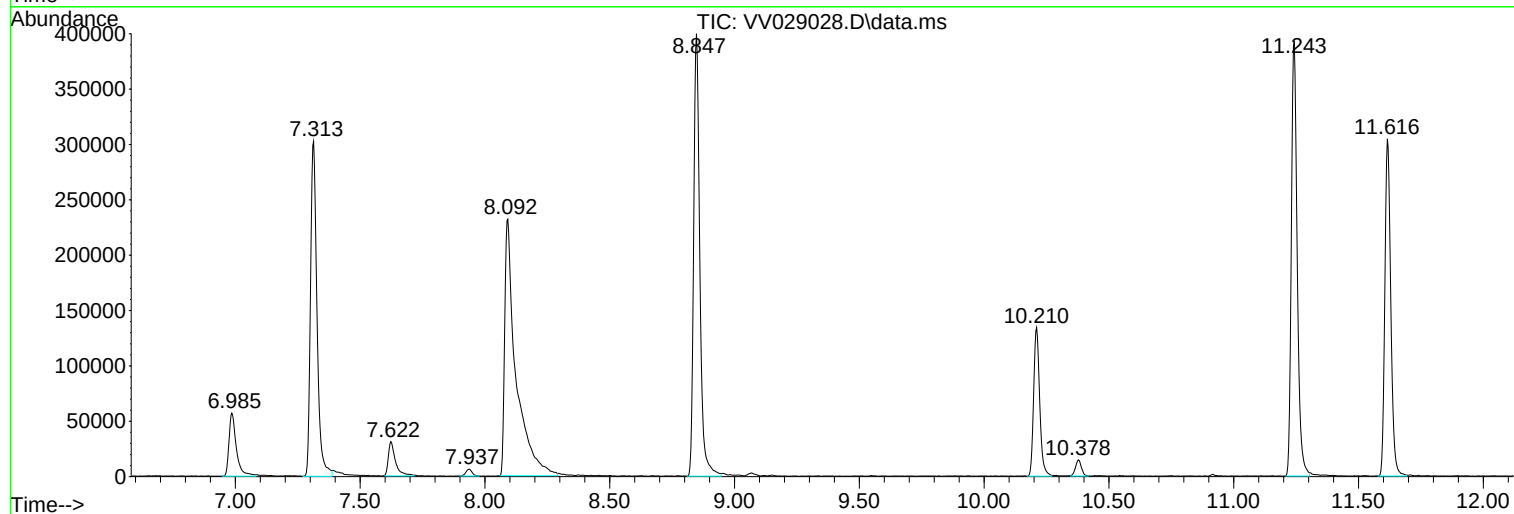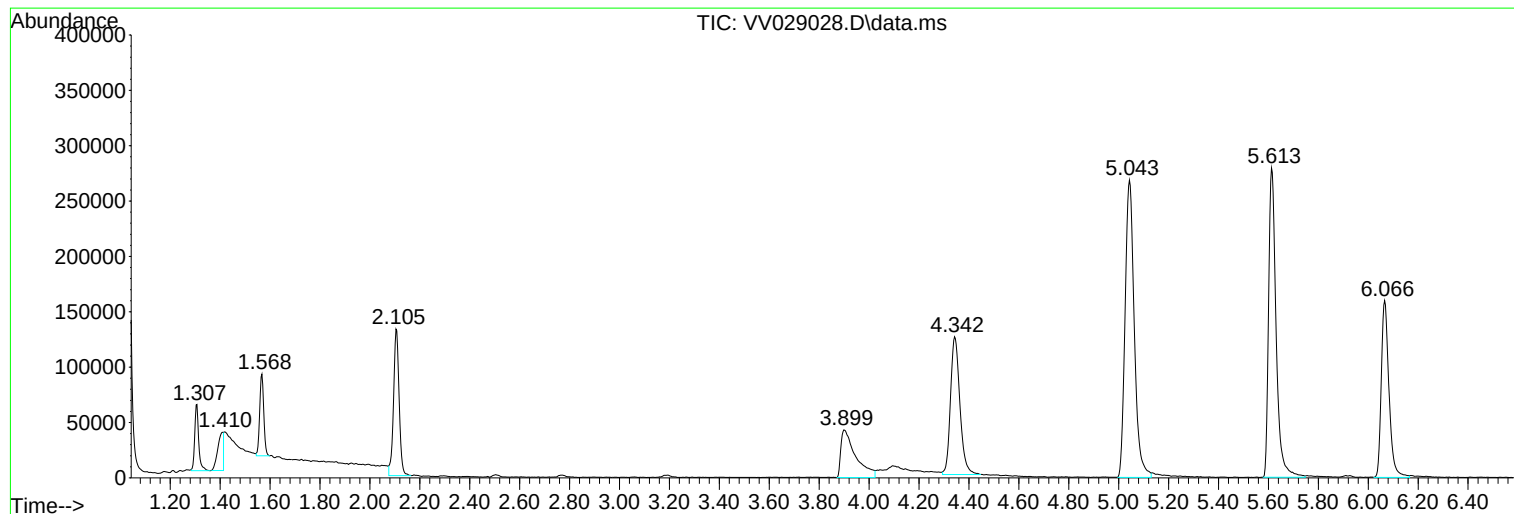

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029028.D
Acq On : 16 Nov 2022 19:42
Operator : SY/MD
Sample : N5620-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029028.D
Acq On : 16 Nov 2022 19:42
Operator : SY/MD
Sample : N5620-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB6

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc