

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029042.D
 Acq On : 17 Nov 2022 01:49
 Operator : SY/MD
 Sample : N5604-17DL 20X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46C1DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029042.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	104	rVB2	126754	142179	15.85%	1.745%
2	1.445	110	126	141	rBV2	30233	135797	15.14%	1.667%
3	1.568	157	164	177	rVB	97908	116427	12.98%	1.429%
4	2.105	321	331	351	rVB	208945	314411	35.05%	3.860%
5	2.503	444	455	473	rBV	102473	171532	19.12%	2.106%
6	2.767	524	537	560	rBV2	37127	80049	8.92%	0.983%
7	3.905	876	891	930	rBV2	274292	817160	91.09%	10.032%
8	4.342	1012	1027	1058	rVB	148370	371670	41.43%	4.563%
9	5.043	1229	1245	1287	rBV2	354704	897121	100.00%	11.013%
10	5.613	1410	1422	1454	rBV	263213	551184	61.44%	6.767%
11	5.915	1504	1516	1536	rBV	68057	143998	16.05%	1.768%
12	6.066	1550	1563	1590	rBV	192323	401505	44.75%	4.929%
13	6.982	1835	1848	1882	rBV	87078	173250	19.31%	2.127%
14	7.310	1938	1950	1976	rBV	448065	807910	90.06%	9.918%
15	7.622	2036	2047	2071	rBV	46372	91686	10.22%	1.126%
16	8.091	2183	2193	2250	rBV2	277608	766050	85.39%	9.404%
17	8.847	2416	2428	2455	rBV	381614	643414	71.72%	7.899%
18	10.210	2839	2852	2876	rBV	143908	237796	26.51%	2.919%
19	11.243	3162	3173	3198	rBV	373478	602428	67.15%	7.396%
20	11.615	3277	3289	3314	rBV	418774	680208	75.82%	8.350%




Sum of corrected areas: 8145775

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029042.D
Acq On : 17 Nov 2022 01:49
Operator : SY/MD
Sample : N5604-17DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46C1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

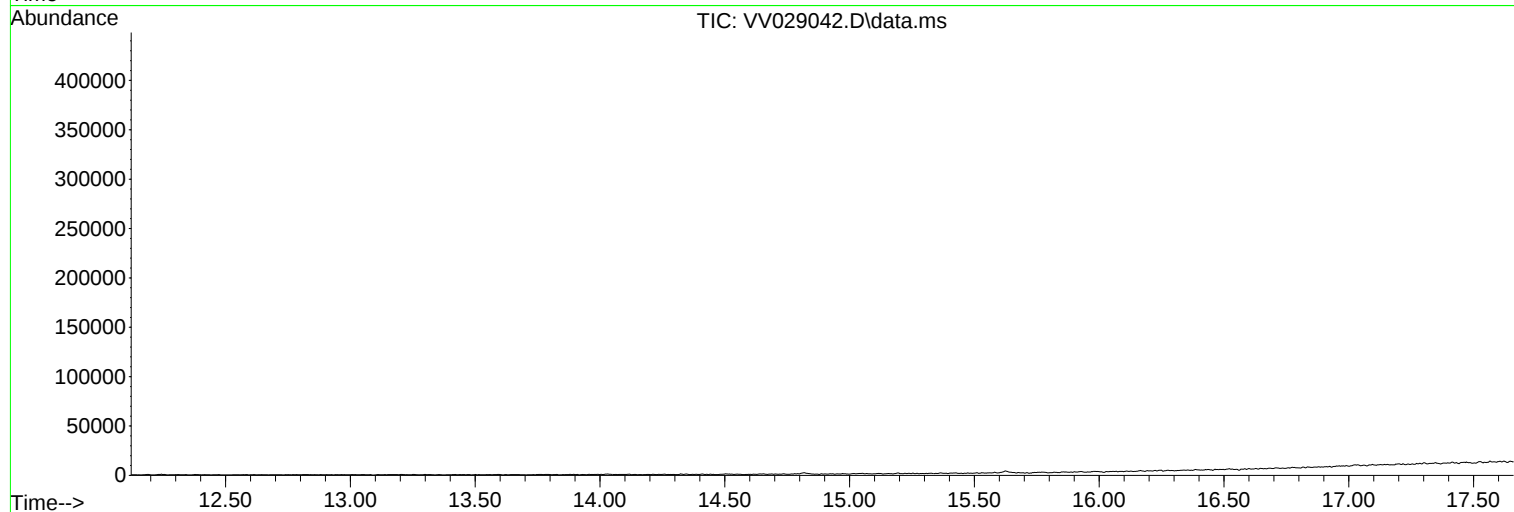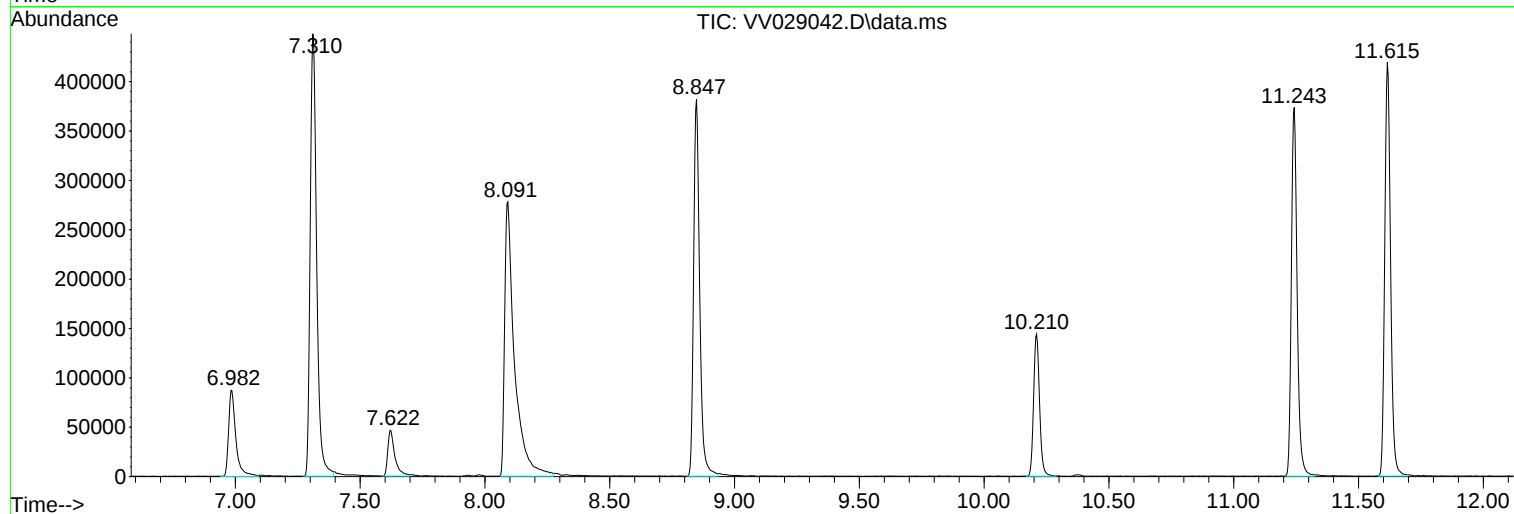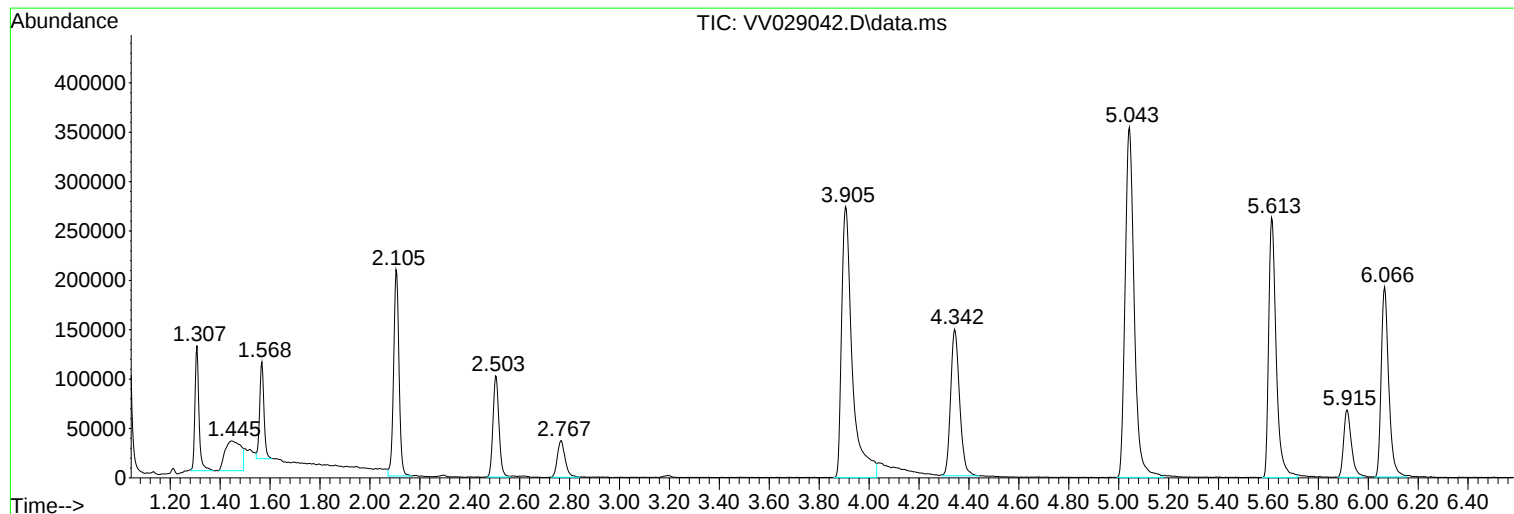

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029042.D
Acq On : 17 Nov 2022 01:49
Operator : SY/MD
Sample : N5604-17DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46C1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029042.D
Acq On : 17 Nov 2022 01:49
Operator : SY/MD
Sample : N5604-17DL 20X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46C1DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc