

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029046.D
 Acq On : 17 Nov 2022 03:27
 Operator : SY/MD
 Sample : N5592-03DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AA8DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029046.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	94	rBV	102164	108664	13.07%	1.331%
2	1.417	109	117	122	rBV	34983	43282	5.21%	0.530%
3	1.458	123	130	133	rVV3	9480	14475	1.74%	0.177%
4	1.568	157	164	178	rVB	91129	109627	13.19%	1.342%
5	2.108	322	332	350	rVB2	212432	333892	40.16%	4.089%
6	2.507	443	456	472	rBV2	47526	81446	9.80%	0.997%
7	3.905	870	891	927	rBV2	55641	243248	29.26%	2.979%
8	4.342	1012	1027	1057	rVB2	138168	353781	42.55%	4.332%
9	5.043	1229	1245	1282	rBV2	328155	831373	100.00%	10.181%
10	5.613	1408	1422	1450	rBV	275985	576153	69.30%	7.055%
11	5.912	1503	1515	1548	rBV	258770	526620	63.34%	6.449%
12	6.066	1550	1563	1595	rVV	179984	373711	44.95%	4.576%
13	6.985	1838	1849	1877	rBV	81744	160084	19.26%	1.960%
14	7.310	1938	1950	1976	rBV	419231	760437	91.47%	9.312%
15	7.622	2037	2047	2067	rBV	42873	83717	10.07%	1.025%
16	7.969	2133	2155	2183	rBV	419213	713001	85.76%	8.731%
17	8.092	2183	2193	2247	rBV3	233253	688567	82.82%	8.432%
18	8.847	2414	2428	2457	rBV	398360	674079	81.08%	8.255%
19	10.210	2840	2852	2879	rVB	134007	219084	26.35%	2.683%
20	11.243	3159	3173	3199	rBV	394142	636855	76.60%	7.799%
21	11.615	3272	3289	3321	rBV	386925	634047	76.27%	7.764%




Sum of corrected areas: 8166143

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029046.D
Acq On : 17 Nov 2022 03:27
Operator : SY/MD
Sample : N5592-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

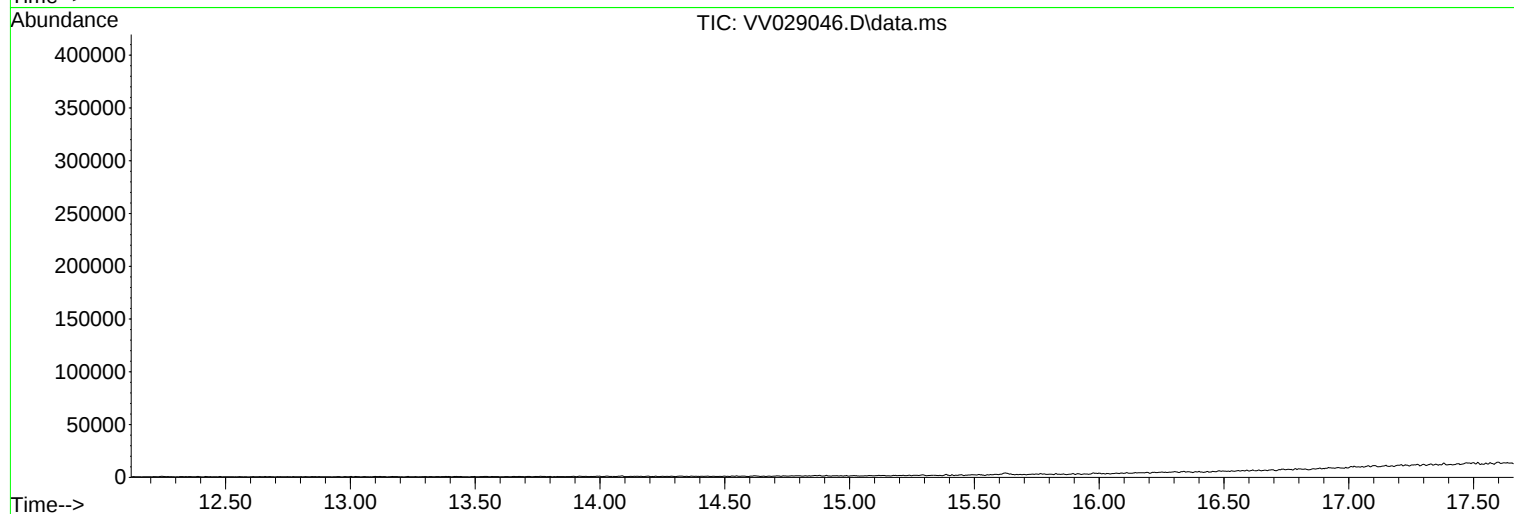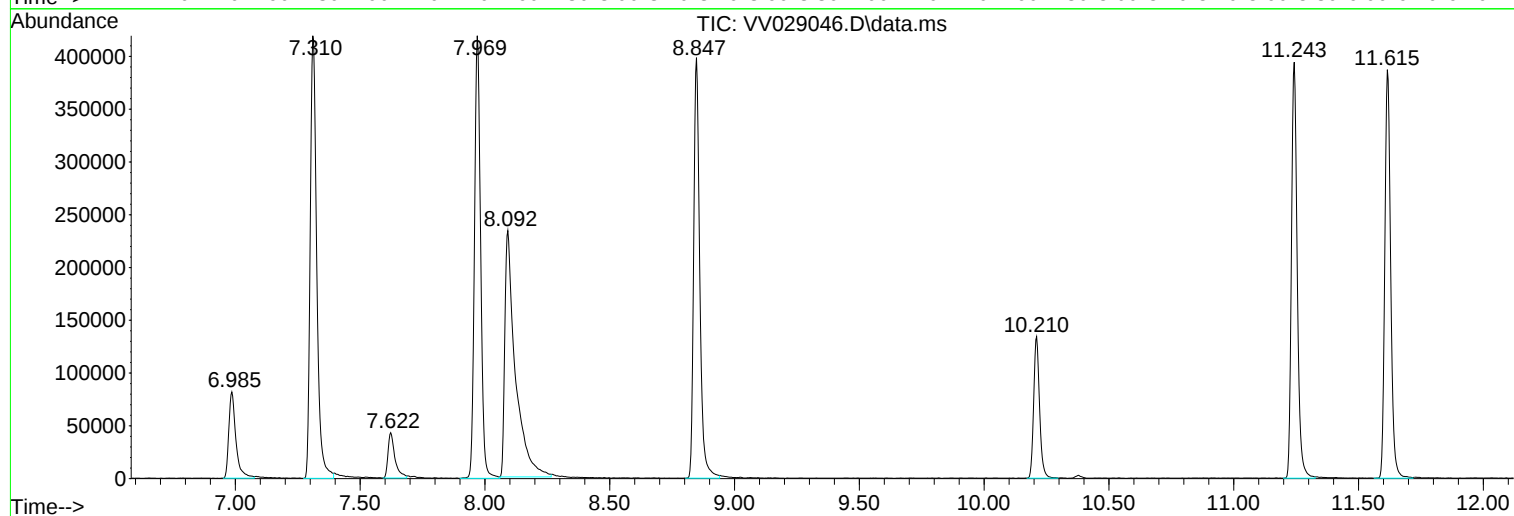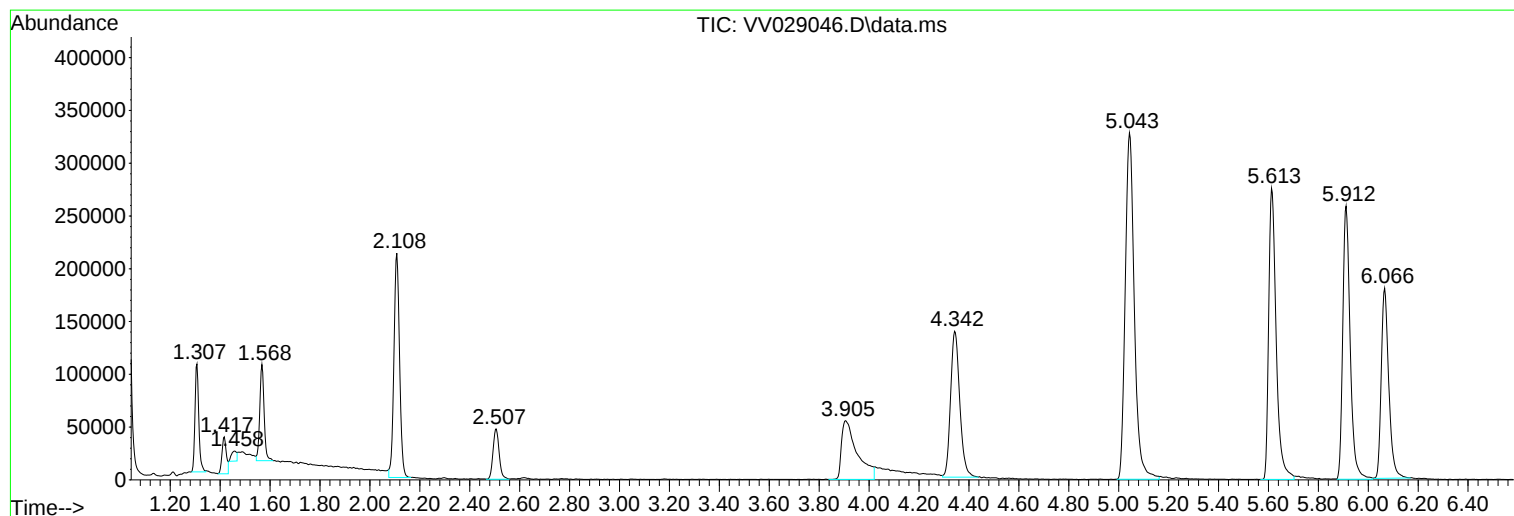

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029046.D
Acq On : 17 Nov 2022 03:27
Operator : SY/MD
Sample : N5592-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029046.D
Acq On : 17 Nov 2022 03:27
Operator : SY/MD
Sample : N5592-03DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 44 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AA8DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc