

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
 Data File : VV029051.D
 Acq On : 17 Nov 2022 05:29
 Operator : SY/MD
 Sample : N5592-12DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AB7DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029051.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	95	rBV	98564	108071	12.74%	1.338%
2	1.420	110	118	120	rBV	22681	27415	3.23%	0.339%
3	1.568	157	164	177	rVB	90419	108124	12.75%	1.339%
4	2.105	321	331	352	rVB2	211827	335134	39.51%	4.150%
5	2.503	442	455	476	rBV	61468	105286	12.41%	1.304%
6	3.188	652	668	684	rBV	15903	34912	4.12%	0.432%
7	3.908	877	892	925	rBV3	99663	352156	41.52%	4.360%
8	4.342	1012	1027	1055	rVB	139769	356080	41.98%	4.409%
9	5.043	1230	1245	1273	rBV2	334814	848158	100.00%	10.502%
10	5.612	1411	1422	1454	rBV	278251	587817	69.31%	7.278%
11	5.911	1504	1515	1545	rBV2	141168	295031	34.78%	3.653%
12	6.066	1550	1563	1595	rBV2	184175	384999	45.39%	4.767%
13	6.985	1835	1849	1868	rBV2	82217	160766	18.95%	1.991%
14	7.310	1938	1950	1975	rBV	428410	777317	91.65%	9.624%
15	7.622	2035	2047	2071	rBV	44183	85830	10.12%	1.063%
16	7.969	2138	2155	2175	rBV	339230	572211	67.47%	7.085%
17	8.091	2182	2193	2240	rBV2	265647	714455	84.24%	8.846%
18	8.847	2416	2428	2464	rBV	409165	691180	81.49%	8.558%
19	10.210	2834	2852	2871	rBV	135293	224321	26.45%	2.777%
20	11.242	3159	3173	3203	rBV	398077	653017	76.99%	8.085%
21	11.615	3276	3289	3308	rBV	400454	654178	77.13%	8.100%




Sum of corrected areas: 8076458

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029051.D
Acq On : 17 Nov 2022 05:29
Operator : SY/MD
Sample : N5592-12DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

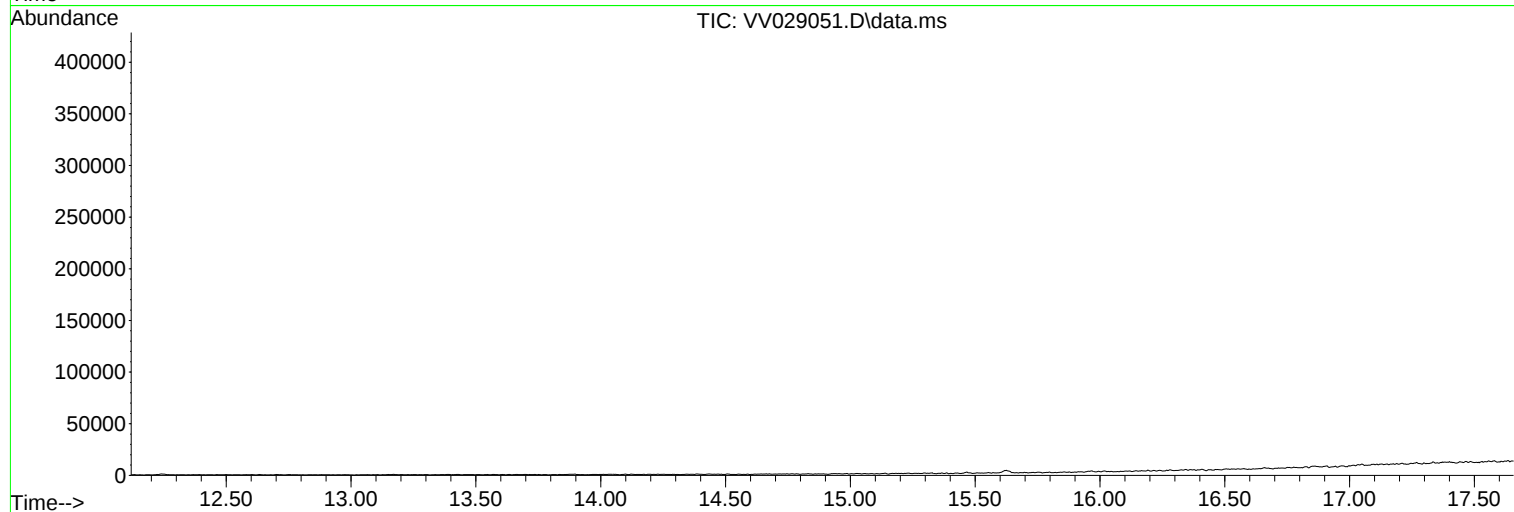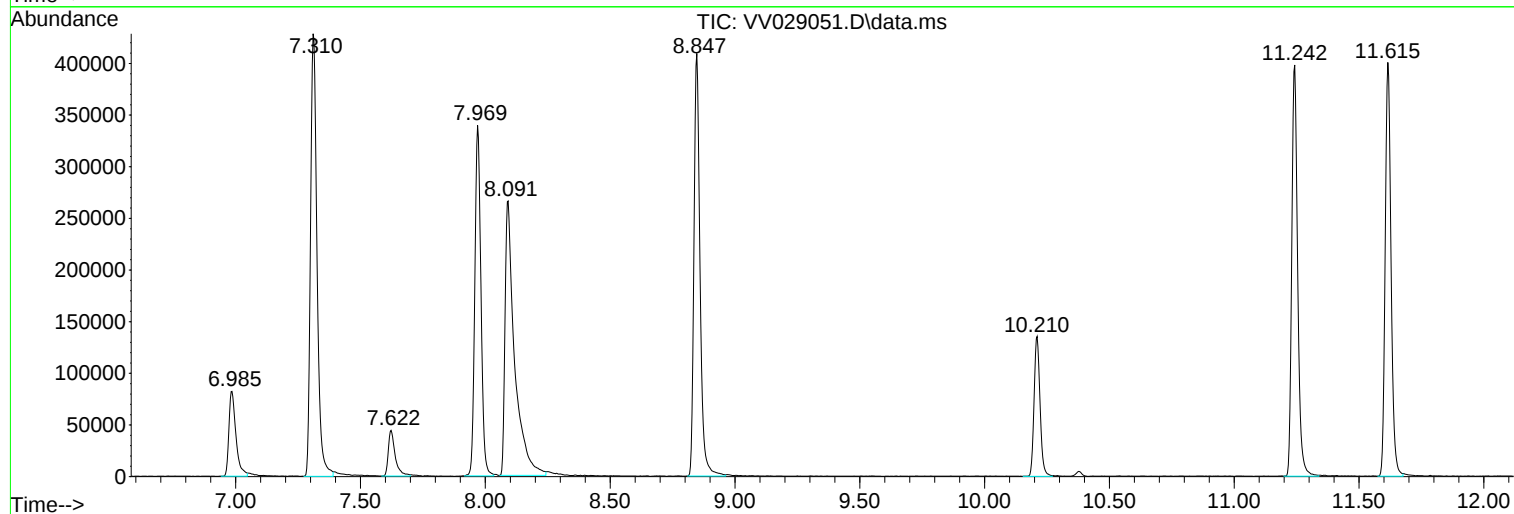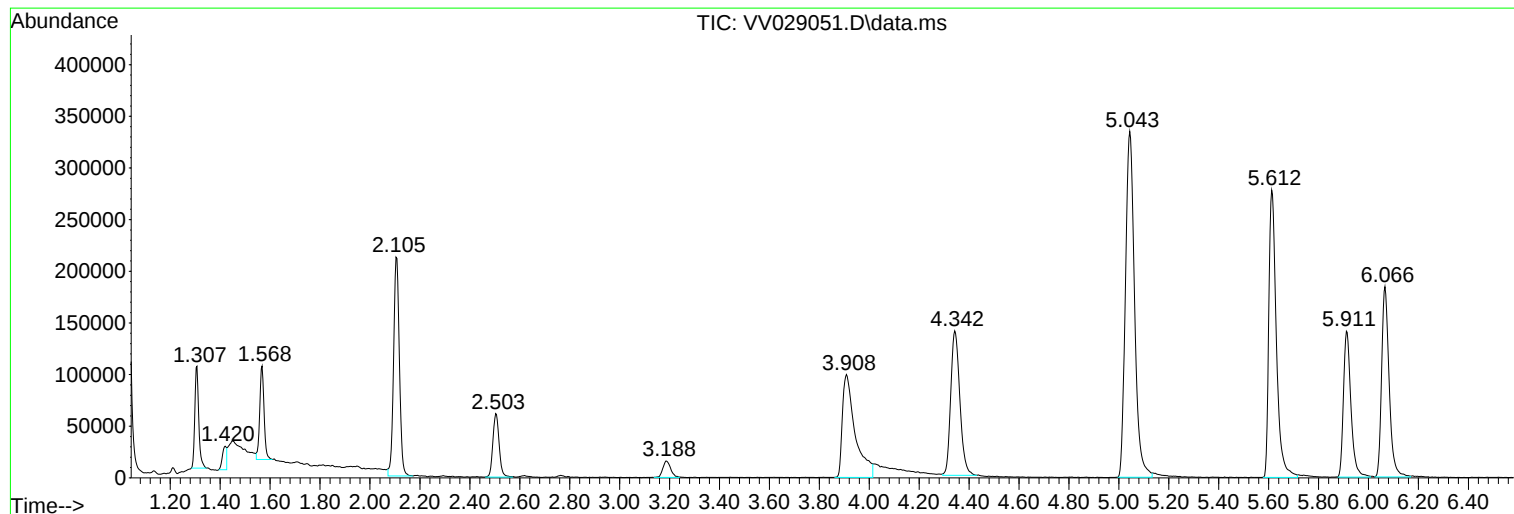

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029051.D
Acq On : 17 Nov 2022 05:29
Operator : SY/MD
Sample : N5592-12DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111622\
Data File : VV029051.D
Acq On : 17 Nov 2022 05:29
Operator : SY/MD
Sample : N5592-12DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 49 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB7DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc