

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111718\
 Data File : VV008587.D
 Acq On : 16 Nov 2018 17:54
 Operator : SY/MD
 Sample : J5987-08
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COL34

Quant Time: Nov 17 04:55:57 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Sat Nov 17 04:38:54 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	157233	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	139728	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	61630	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	30652	4.39	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	87.80%
7) Chloroethane-d5	1.59	69	23800	4.14	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	82.80%
11) 1,1-Dichloroethene-d2	2.14	63	44852	3.17	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	63.40%
20) 2-Butanone-d5	3.96	46	111802	44.74	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	89.48%
24) Chloroform-d	4.41	84	76930	4.03	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	80.60%
26) 1,2-Dichloroethane-d4	5.09	65	42054	4.33	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	86.60%
32) Benzene-d6	5.10	84	156654	4.30	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	86.00%
36) 1,2-Dichloropropane-d6	6.12	67	51426	4.37	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	87.40%
41) Toluene-d8	7.36	98	145265	4.24	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	84.80%
43) trans-1,3-Dichloropropene-	7.67	79	18234	4.07	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	81.40%
46) 2-Hexanone-d5	8.14	63	85808	42.25	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	84.50%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	34638	4.22	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	84.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	47280	4.25	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	85.00%


Target Compounds					Qvalue
13) Acetone	2.21	43	30098	23.094 ug/L	94
30) Cyclohexane	4.73	56	66497	3.390 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111718\
Data File : VV008587.D
Acq On : 16 Nov 2018 17:54
Operator : SY/MD
Sample : J5987-08
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
COL34

Quant Time: Nov 17 04:55:57 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Sat Nov 17 04:38:54 2018
Response via : Initial Calibration

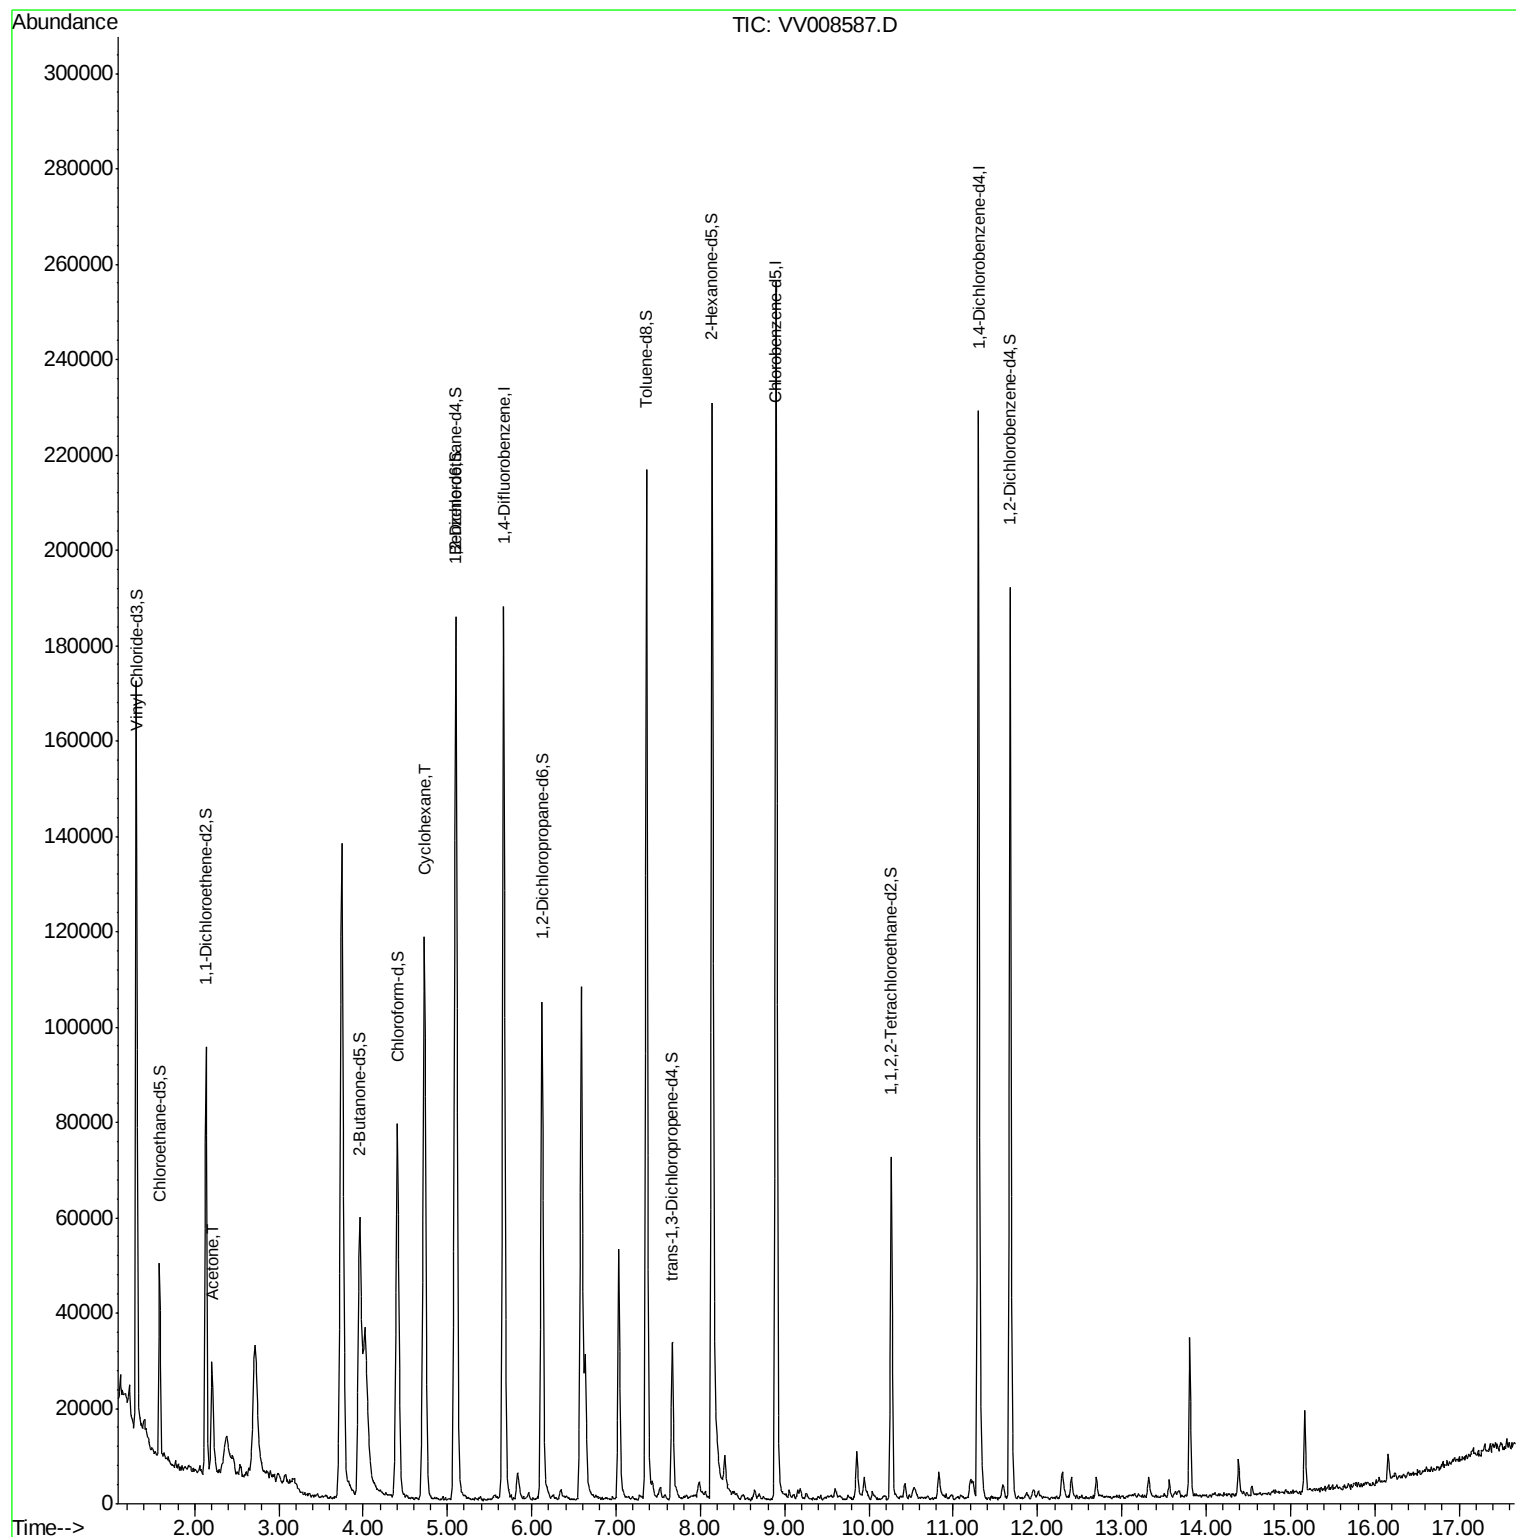

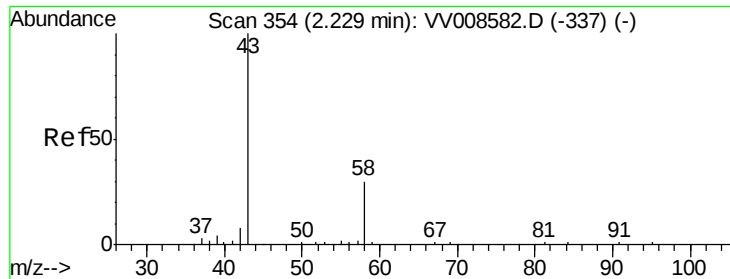

#13

Acetone

Concen: 23.094 ug/L

RT: 2.21 min Scan# 348

Delta R.T. -0.02 min

Lab File: VV008587.D

Acq: 16 Nov 2018 17:54

Instrument :

MSVOA_V

ClientSampleId :


COL34

Tgt Ion: 43 Resp: 30098

Ion Ratio Lower Upper

43 100

58 31.5 0.0 56.4

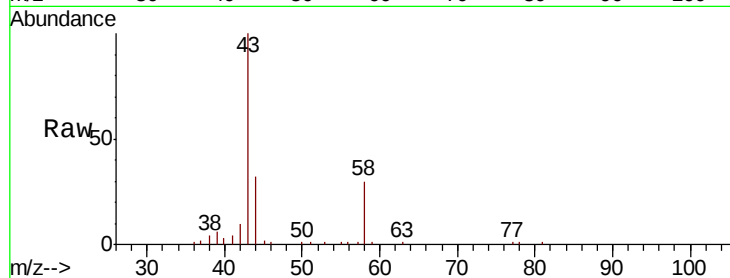

Abundance Ion 43.05 (42.75 to 43.75): VV008587.D (-348) (-)

Ion 58.05 (57.75 to 58.75): VV008587.D (-348) (-)

2.21

15000



10000

5000

0

2.15 2.20 2.25 2.30

Time-->

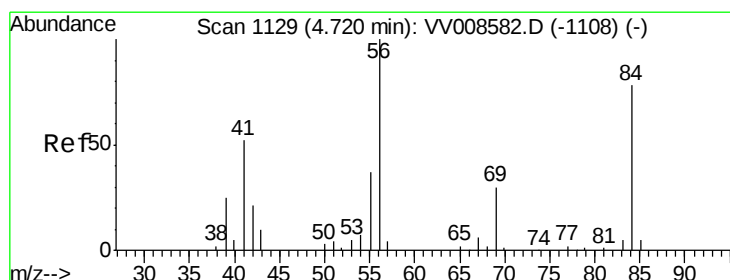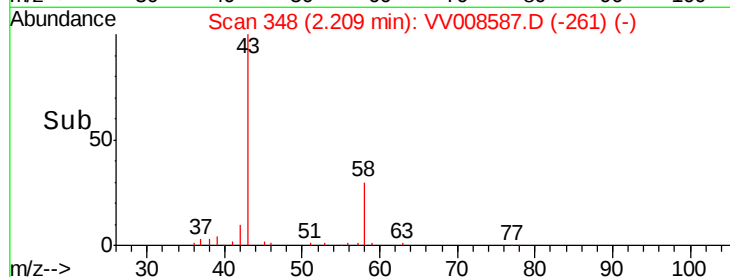

#30

Cyclohexane

Concen: 3.390 ug/L

RT: 4.73 min Scan# 1131

Delta R.T. 0.01 min

Lab File: VV008587.D

Acq: 16 Nov 2018 17:54


Tgt Ion: 56 Resp: 66497

Ion Ratio Lower Upper

56 100

69 30.2 24.2 36.4

84 81.8 65.7 98.5

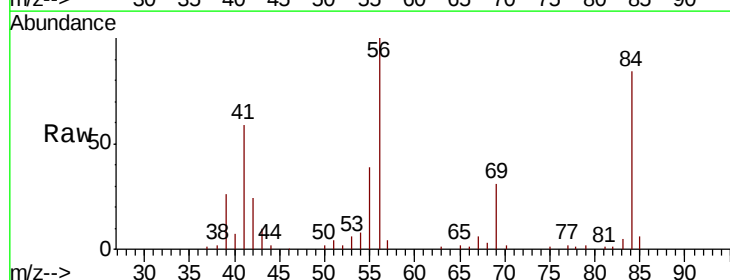

Abundance Ion 56.10 (55.80 to 56.80): VV008587.D (-1131) (-)

Ion 69.15 (68.85 to 69.85): VV008587.D (-1131) (-)

Ion 84.15 (83.85 to 84.85): VV008587.D (-1131) (-)

4.73

30000

20000

10000

0

4.65 4.70 4.75 4.80

Time-->

