


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111718\
Data File : VV008579.D
Acq On : 16 Nov 2018 14:08
Operator : SY/MD
Sample : BFB48
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB48

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
Title : TRACE VOA SOM01.0
Last Update : Mon Nov 19 02:55:31 2018

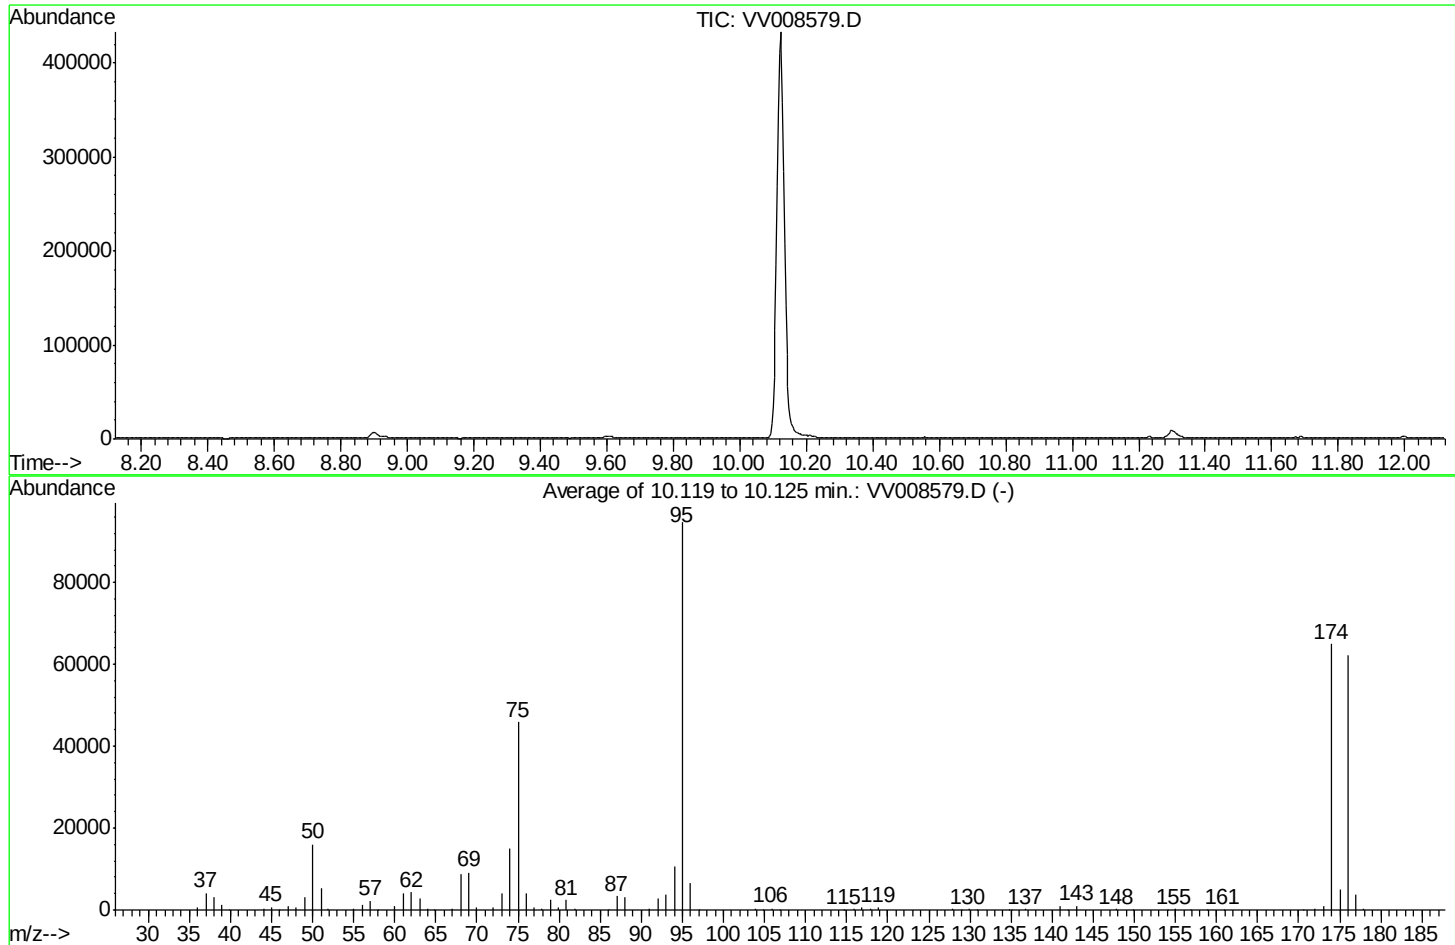

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2795

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	16074	PASS
75	95	30	80	48.5	45949	PASS
95	95	100	100	100.0	94685	PASS
96	95	5	9	6.8	6477	PASS
173	174	0.00	2	1.5	981	PASS
174	95	50	120	68.6	64965	PASS
175	174	5	9	7.7	5017	PASS
176	174	95	101	95.6	62114	PASS
177	176	5	9	6.2	3880	PASS

m/z	Abundance
36.00	677.0
37.00	4141.0
38.00	3368.0
39.00	1334.0
39.90	378.0
41.10	110.0
44.00	1018.0
45.00	788.0
47.00	999.0
48.00	452.0
49.00	3307.0
50.00	15716.0
51.00	5270.0
51.90	262.0
54.90	257.0
56.00	1185.0
57.00	2200.0
57.90	154.0
60.00	819.0
61.00	3901.0
62.00	4228.0
63.10	2811.0
64.00	308.0
64.90	128.0
66.90	252.0
68.00	8952.0
69.00	9535.0
70.00	609.0
72.00	561.0
73.00	3856.0
74.00	14840.0
75.00	45392.0
76.00	4159.0
77.00	558.0
77.80	308.0
78.90	2302.0
79.90	714.0
80.90	2295.0
81.90	428.0
85.90	111.0
87.00	3129.0
88.00	3386.0
90.90	404.0
92.00	2709.0
93.00	3647.0
94.00	10258.0
95.00	93272.0
96.00	6563.0
97.00	175.0
103.90	355.0
104.80	181.0
105.90	377.0
114.70	143.0
115.90	425.0
116.90	455.0
117.90	315.0
118.80	536.0
127.90	245.0
128.90	106.0
129.80	251.0
130.80	120.0
134.80	104.0
136.70	177.0
140.90	720.0
142.00	188.0
143.00	942.0
147.90	237.0
154.00	114.0
154.90	228.0
160.90	159.0
170.50	104.0
171.90	340.0
173.10	1002.0
174.00	62264.0
175.00	4774.0
176.00	59264.0
177.00	3781.0
177.90	172.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
38.90	122.0
39.80	325.0
41.10	104.0
44.00	585.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	633.0
37.00	3836.0
38.00	2994.0
39.00	1234.0
39.90	477.0
44.00	974.0
45.00	657.0
46.00	114.0
47.00	1059.0
48.00	487.0
49.00	3010.0
50.00	15851.0
51.00	4913.0
51.90	222.0
54.90	262.0
56.00	1117.0
57.00	2203.0
58.10	114.0
60.00	793.0
61.00	3895.0
62.00	4160.0
63.00	2826.0
63.90	237.0
64.80	164.0
66.90	235.0
68.00	8600.0
69.00	8663.0
69.90	712.0
71.90	591.0
73.00	4090.0
74.00	14442.0
75.00	44952.0
76.00	3990.0
77.00	484.0
77.90	401.0
78.90	2376.0
79.90	744.0
80.90	2437.0
81.80	510.0
87.00	3565.0
87.90	2892.0
90.90	339.0
92.00	2514.0
93.00	3604.0
94.00	10827.0
95.00	92592.0
96.00	6144.0
97.00	142.0
103.90	298.0
104.90	108.0
105.80	368.0
106.90	113.0
114.70	140.0
115.90	361.0
116.80	514.0
117.90	304.0
118.90	463.0
127.90	289.0
128.90	147.0
129.90	329.0
130.90	188.0
135.00	133.0
136.90	205.0
140.90	842.0
141.80	145.0
143.00	1062.0
147.80	223.0
149.90	103.0
154.90	222.0
156.90	138.0
158.90	101.0
172.10	356.0
173.00	921.0
174.00	65480.0
175.00	5099.0
176.00	62736.0
177.00	3884.0
177.90	167.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48

m/z	Abundance
36.00	652.0
37.00	4254.0
38.00	3378.0
39.00	1323.0
39.90	413.0
41.10	124.0
44.00	1027.0
45.00	698.0
47.00	1072.0
48.00	518.0
49.00	3265.0
50.00	16656.0
51.00	5410.0
51.90	269.0
54.90	267.0
56.00	1168.0
57.00	2279.0
58.00	131.0
60.00	841.0
61.00	3994.0
62.00	4477.0
63.00	2961.0
63.90	261.0
64.90	147.0
66.90	282.0
68.00	9164.0
69.00	9452.0
69.90	686.0
71.90	597.0
73.00	4226.0
74.00	15349.0
75.00	47504.0
76.00	4285.0
77.00	502.0
77.90	333.0
78.90	2492.0
79.90	789.0
80.90	2466.0
81.80	470.0
85.90	107.0
87.00	3403.0
88.00	3298.0
90.90	411.0
92.00	2791.0
93.00	3852.0
94.00	11001.0
95.00	98192.0
96.00	6726.0
97.00	151.0
103.90	338.0
104.80	166.0
105.90	387.0
114.70	171.0
115.90	441.0
116.80	477.0
117.90	321.0
118.80	554.0
127.90	303.0
128.90	138.0
129.80	302.0
130.90	158.0
136.80	192.0
140.90	841.0
141.90	152.0
143.00	1060.0
147.80	230.0
154.00	110.0
154.90	241.0
156.90	106.0
160.90	148.0
172.00	384.0
173.00	1021.0
174.00	67152.0
175.00	5179.0
176.00	64344.0
177.00	3976.0
177.80	196.0

Instrument :
MSVOA_V
ClientSampleId :
BFB48