


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV111720\
 Data File : VV019379.D
 Acq On : 17 Nov 2020 08:58
 Operator : SY/MD
 Sample : BFB95
 Misc : 5.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB95

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVLM111220WMA.M
 Title : VOC Analysis
 Last Update : Tue Nov 17 17:05:19 2020

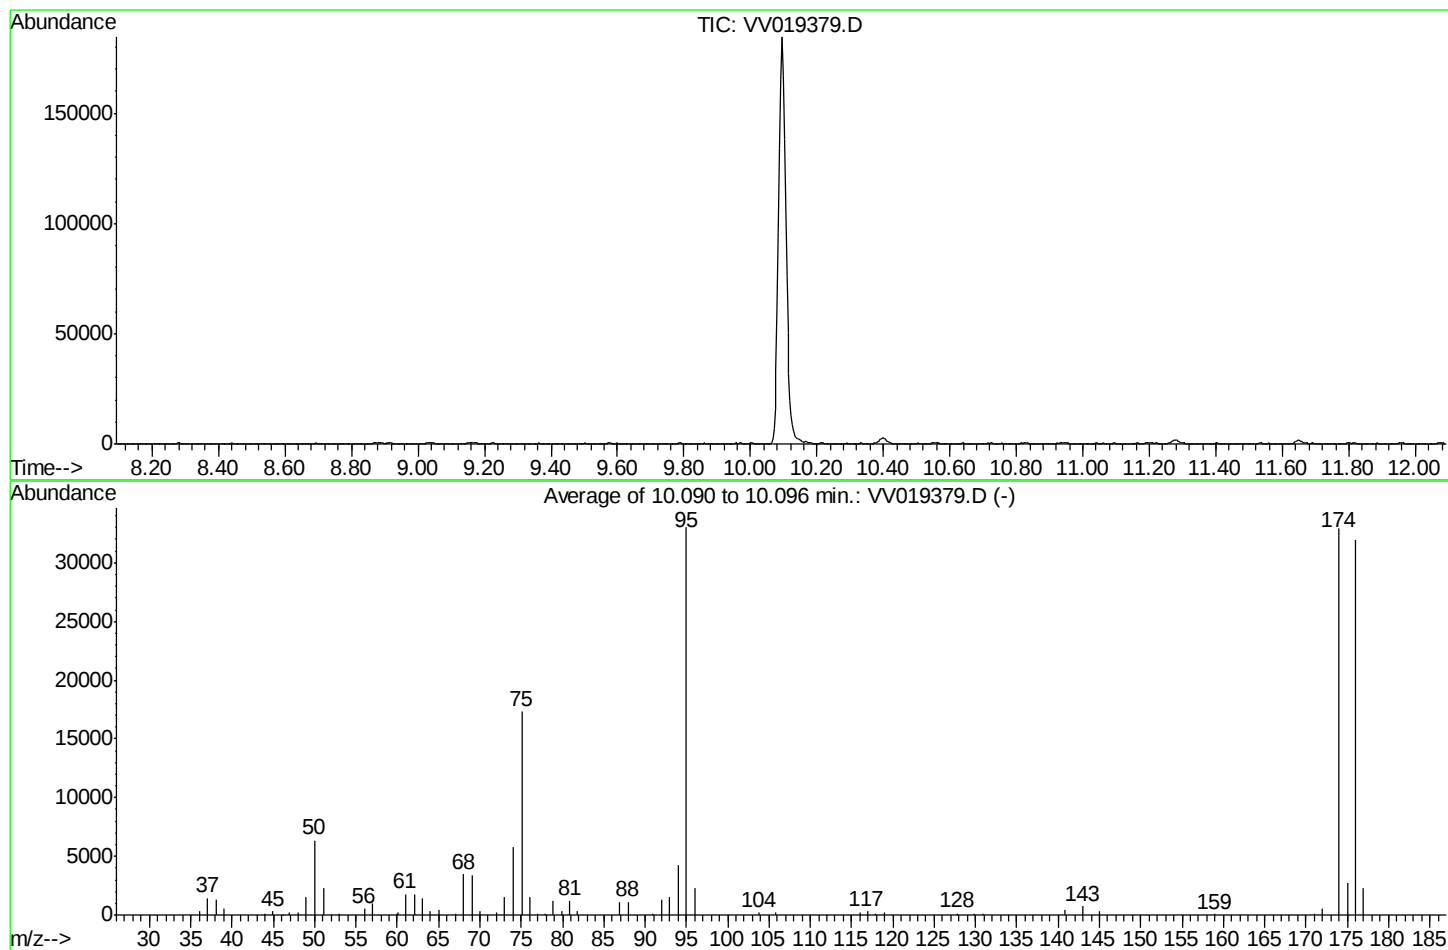

AutoFind: Scans 2799, 2800, 2801; Background Corrected with Scan 2789

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	6360	PASS
75	95	30	80	52.5	17326	PASS
95	95	100	100	100.0	33016	PASS
96	95	5	9	7.1	2344	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	99.6	32888	PASS
175	174	5	9	8.2	2710	PASS
176	174	95	101	97.3	31984	PASS
177	176	5	9	7.2	2298	PASS

m/z	Abundance
36.00	325.0
37.00	1448.0
38.00	1284.0
39.00	556.0
44.00	247.0
45.00	325.0
46.20	112.0
46.90	250.0
48.00	251.0
49.00	1409.0
50.00	5951.0
51.10	2081.0
52.00	112.0
52.90	118.0
55.90	442.0
57.00	1020.0
59.90	322.0
61.00	1709.0
62.10	1624.0
63.00	1403.0
64.00	287.0
65.00	396.0
68.00	3327.0
69.10	3297.0
70.10	267.0
71.90	154.0
73.00	1495.0
74.10	5408.0
75.10	16299.0
76.00	1360.0
76.90	118.0
77.90	171.0
78.90	1062.0
79.90	351.0
80.90	1199.0
81.80	280.0
87.00	1021.0
88.00	1166.0
91.90	1177.0
93.00	1402.0
94.00	3814.0
95.00	31136.0
96.00	2323.0
103.80	204.0
105.90	118.0
116.00	224.0
116.90	287.0
117.90	147.0
119.00	188.0
127.80	112.0
129.80	103.0
140.80	422.0
143.00	722.0
145.00	280.0
171.00	127.0
172.00	508.0
174.00	29560.0
175.00	2581.0
176.00	29216.0
177.00	2158.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.00	324.0
37.10	1439.0
38.00	1307.0
39.10	573.0
44.00	216.0
45.00	298.0
46.90	279.0
47.90	251.0
49.00	1555.0
50.00	6517.0
51.00	2412.0
52.90	102.0
56.00	522.0
57.00	1070.0
60.10	348.0
61.00	1785.0
62.00	1812.0
63.00	1498.0
63.90	294.0
65.00	435.0
67.00	113.0
68.00	3575.0
69.10	3506.0
70.00	298.0
72.00	196.0
73.00	1658.0
74.00	6070.0
75.10	17856.0
76.00	1529.0
76.90	147.0
77.90	161.0
78.90	1255.0
79.90	359.0
80.90	1282.0
81.80	331.0
86.90	1138.0
87.90	1180.0
90.90	109.0
91.90	1314.0
93.00	1536.0
94.00	4311.0
95.00	34096.0
96.00	2478.0
103.80	186.0
105.80	185.0
116.00	234.0
116.90	340.0
117.90	170.0
118.90	228.0
127.80	126.0
129.90	106.0
130.90	110.0
140.90	485.0
143.00	769.0
145.00	298.0
159.00	110.0
171.00	131.0
171.90	590.0
174.00	33992.0
175.00	2792.0
176.00	33128.0
177.00	2392.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
36.00	292.0
37.10	1428.0
38.10	1287.0
39.10	553.0
44.00	222.0
44.90	277.0
47.00	280.0
48.00	240.0
49.00	1535.0
50.00	6612.0
51.00	2328.0
53.00	103.0
56.10	526.0
57.00	1008.0
60.00	401.0
61.00	1780.0
62.00	1781.0
63.00	1502.0
63.90	280.0
65.00	367.0
67.00	121.0
68.00	3451.0
69.10	3426.0
70.00	321.0
72.00	271.0
73.00	1587.0
74.00	5994.0
75.10	17824.0
76.00	1547.0
76.90	159.0
77.90	123.0
78.90	1348.0
80.00	338.0
80.90	1240.0
81.80	325.0
86.90	1173.0
87.90	1086.0
90.90	116.0
92.00	1294.0
93.00	1564.0
94.00	4562.0
95.00	33816.0
96.00	2233.0
103.90	152.0
105.80	232.0
115.90	182.0
116.90	317.0
117.90	160.0
118.90	269.0
127.90	141.0
129.90	138.0
130.90	101.0
140.90	475.0
143.00	732.0
145.00	278.0
159.00	106.0
171.00	129.0
172.00	614.0
174.00	35112.0
175.00	2759.0
176.00	33608.0
177.00	2345.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95

m/z	Abundance
43.90	160.0

Instrument :
MSVOA_V
ClientSampleId :
BFB95