


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023577.D
Acq On : 17 Nov 2021 18:11
Operator : SY/MD
Sample : M4617-07
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Nov 18 00:23:28 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Nov 18 00:20:29 2021
Response via : Initial Calibration

Reviewed By :John Carlone 11/18/2021
Supervised By :Mahesh Dadoda 11/18/2021

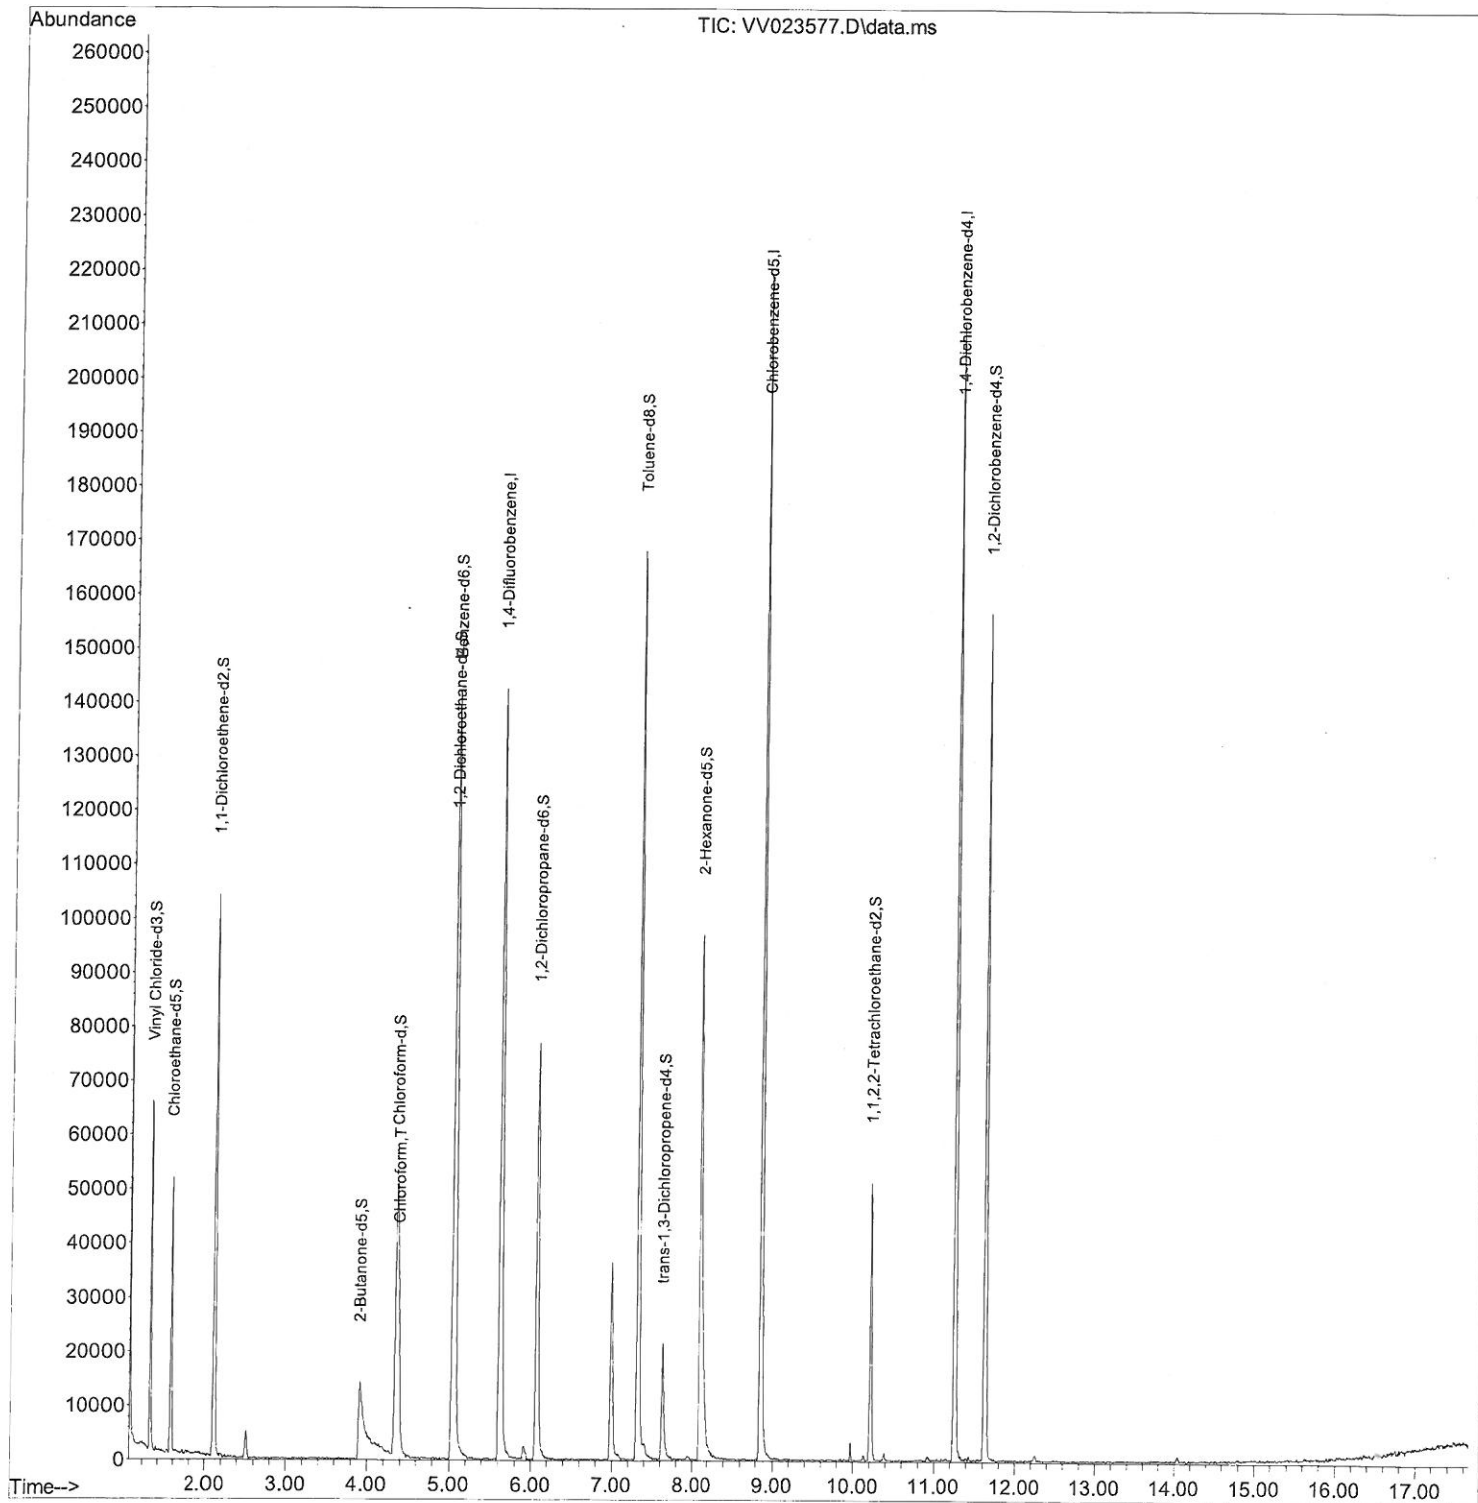

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
 Data File : VV023577.D
 Acq On : 17 Nov 2021 18:11
 Operator : SY/MD
 Sample : M4617-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Nov 18 00:23:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 18 00:20:29 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/18/2021
 Supervised By :Mahesh Dadoda 11/18/2021

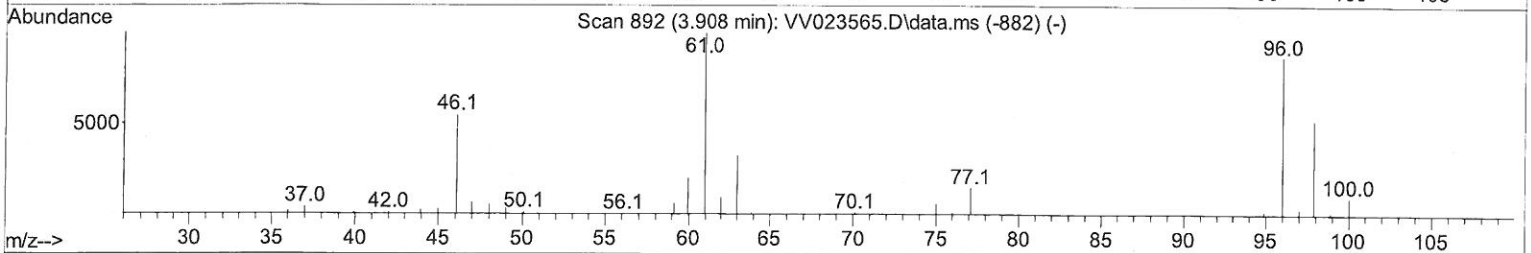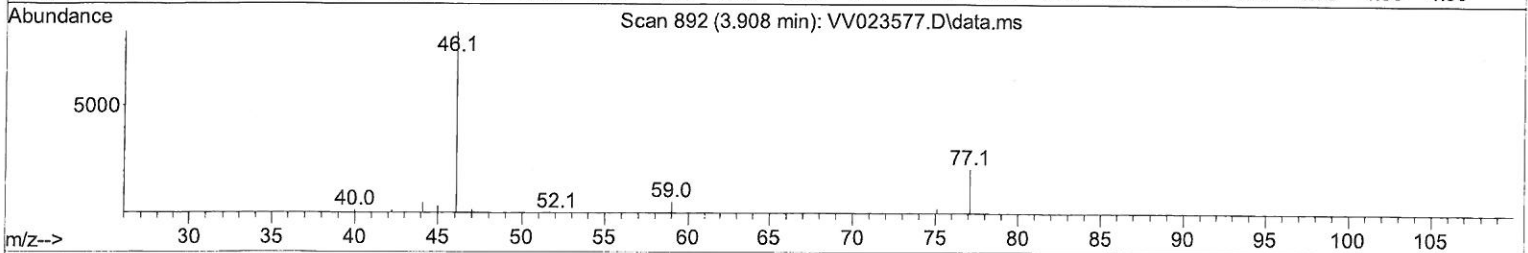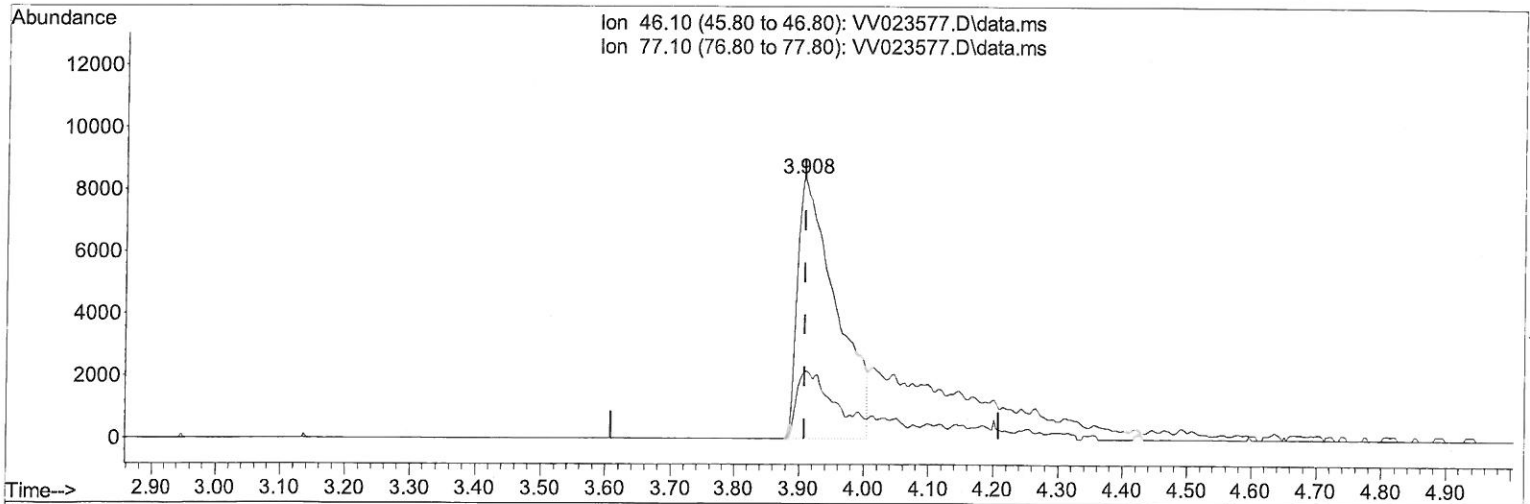

TIC: VV023577.D\data.ms

(20) 2-Butanone-d5 (S)

3.908min (+ 0.000) 24.95 ug/L

response 34393

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	10.44#
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
 Data File : VV023577.D
 Acq On : 17 Nov 2021 18:11
 Operator : SY/MD
 Sample : M4617-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Nov 18 00:23:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 18 00:20:29 2021
 Response via : Initial Calibration

Reviewed By :John Carlone 11/18/2021
 Supervised By :Mahesh Dadoda 11/18/2021

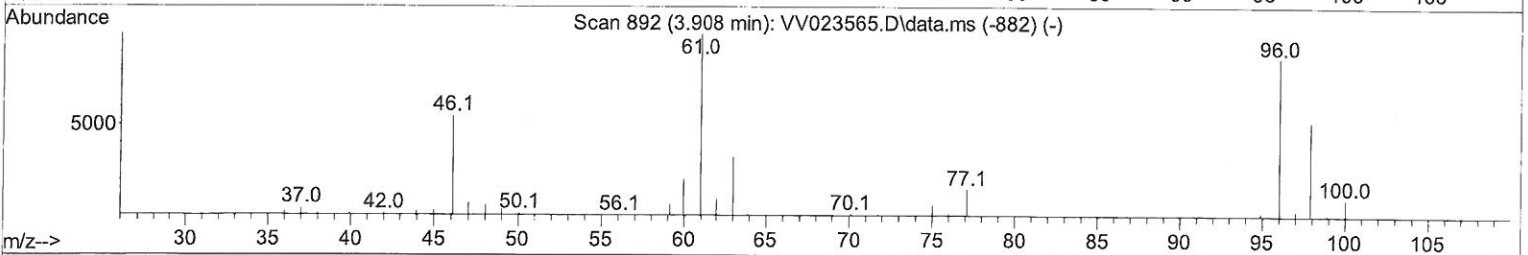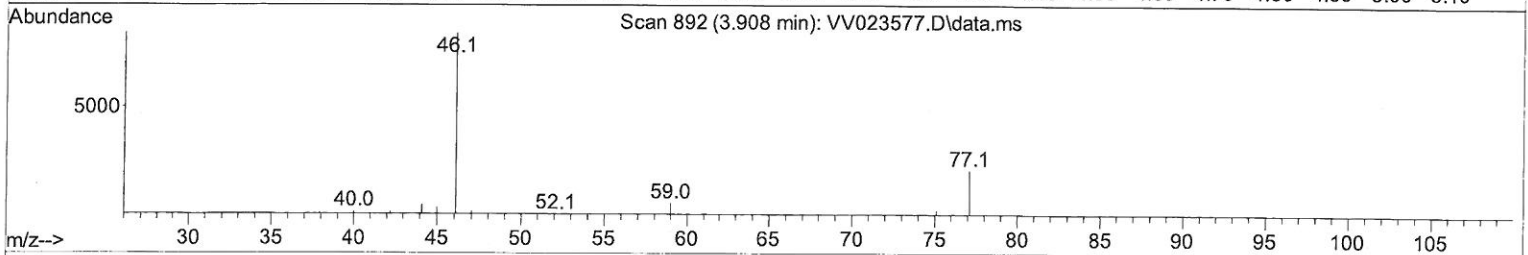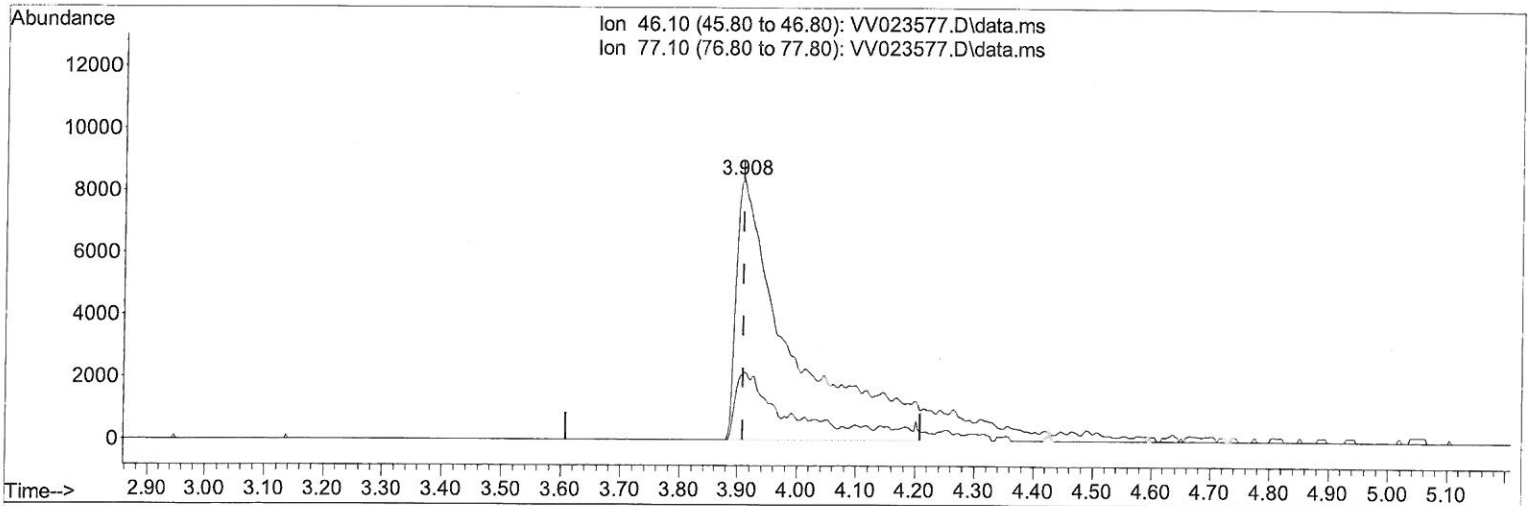

TIC: VV023577.D\data.ms

(20) 2-Butanone-d5 (S)

3.908min (+ 0.000) 39.30 ug/L m

response 54163

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	22.30	6.63#
0.00	0.00	0.00
0.00	0.00	0.00

7 MD
11/20/21

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111721\
 Data File : VW023577.D
 Acq On : 17 Nov 2021 18:11
 Operator : SY/MD
 Sample : M4617-07
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual Integrations APPROVED

Reviewed By : John Carlone 11/18/2021
 Supervised By : Mahesh Dadoda 11/18/2021

Quant Time: Nov 18 00:23:28 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Nov 18 00:20:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.619	114	127708	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.853	117	123234	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.249	152	57017	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	38675	4.834	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	96.600%		
7) Chloroethane-d5	1.568	69	29676	4.551	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	91.000%		
11) 1,1-Dichloroethene-d2	2.108	63	53563	3.576	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	71.600%		
20) 2-Butanone-d5	3.908	46	54163m	39.296	ug/L	0.00
Spiked Amount 50.000	Range 40 - 130		Recovery =	78.600%		
24) Chloroform-d	4.352	84	44508	2.610	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	52.200%#		
26) 1,2-Dichloroethane-d4	5.037	65	31353	4.089	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	81.800%		
32) Benzene-d6	5.053	84	129909	4.109	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	82.200%		
36) 1,2-Dichloropropane-d6	6.072	67	36724	3.945	ug/L	0.00
Spiked Amount 5.000	Range 60 - 140		Recovery =	79.000%		
41) Toluene-d8	7.317	98	114623	3.868	ug/L	0.00
Spiked Amount 5.000	Range 70 - 130		Recovery =	77.400%		
43) trans-1,3-Dichloroprop...	7.625	79	13382	3.792	ug/L	0.00
Spiked Amount 5.000	Range 55 - 130		Recovery =	75.800%		
46) 2-Hexanone-d5	8.095	63	41419	31.896	ug/L	0.00
Spiked Amount 50.000	Range 45 - 130		Recovery =	63.800%		
56) 1,1,2,2-Tetrachloroeth...	10.217	84	23725	3.544	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	70.800%		
66) 1,2-Dichlorobenzene-d4	11.625	152	42785	4.507	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	90.200%		
Target Compounds						
25) Chloroform	4.378	83	22084	1.311	ug/L	88

7m8
11/26/21

(#) = qualifier out of range (m) = manual integration (+) = signals summed