

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
 Data File : VV023567.D
 Acq On : 17 Nov 2021 14:13
 Operator : SY/MD
 Sample : M4643-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 GB8K1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023567.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.214	50	54	62	rBV	4738	4330	1.03%	0.141%
2	1.294	71	79	95	rBV2	389443	419490	100.00%	13.693%
3	1.568	156	164	177	rVB	36871	41016	9.78%	1.339%
4	1.908	263	270	280	rVB2	3034	4914	1.17%	0.160%
5	2.108	321	332	348	rVB	68561	99954	23.83%	3.263%
6	2.507	447	456	465	rBV2	8323	14045	3.35%	0.458%
7	3.921	883	896	925	rBV	14623	67039	15.98%	2.188%
8	4.349	1013	1029	1054	rVB2	55731	149118	35.55%	4.868%
9	5.047	1229	1246	1269	rBV2	120665	305721	72.88%	9.979%
10	5.616	1409	1423	1449	rBV	122170	254797	60.74%	8.317%
11	5.912	1507	1515	1526	rBV4	2393	4386	1.05%	0.143%
12	6.072	1553	1565	1584	rBV	70620	147489	35.16%	4.814%
13	6.584	1715	1724	1734	rBV6	2407	4819	1.15%	0.157%
14	6.989	1840	1850	1875	rBV	34018	67861	16.18%	2.215%
15	7.317	1941	1952	1970	rBV	139492	248759	59.30%	8.120%
16	7.625	2039	2048	2064	rBV2	19004	35819	8.54%	1.169%
17	8.095	2183	2194	2235	rBV2	104550	274392	65.41%	8.957%
18	8.854	2419	2430	2452	rBV	190718	316936	75.55%	10.345%
19	10.217	2844	2854	2867	rBV	51163	82860	19.75%	2.705%
20	11.249	3164	3175	3202	rBV	184256	287170	68.46%	9.374%
21	11.625	3278	3292	3308	rBV	145845	232604	55.45%	7.593%




Sum of corrected areas: 3063519

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023567.D
Acq On : 17 Nov 2021 14:13
Operator : SY/MD
Sample : M4643-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

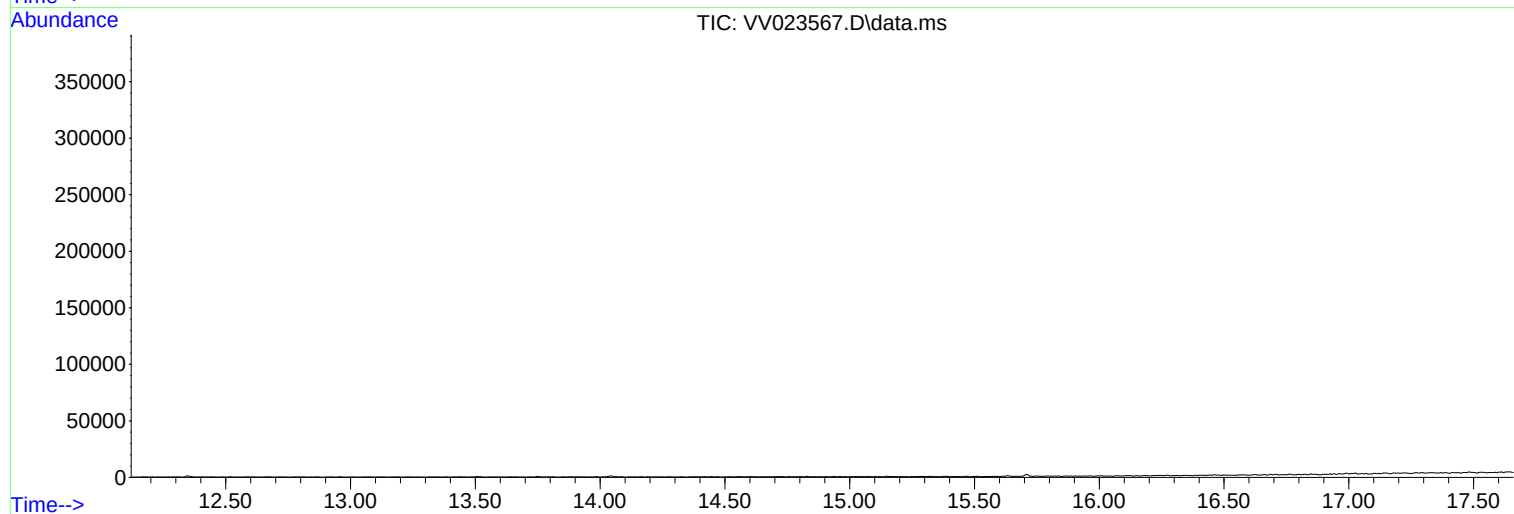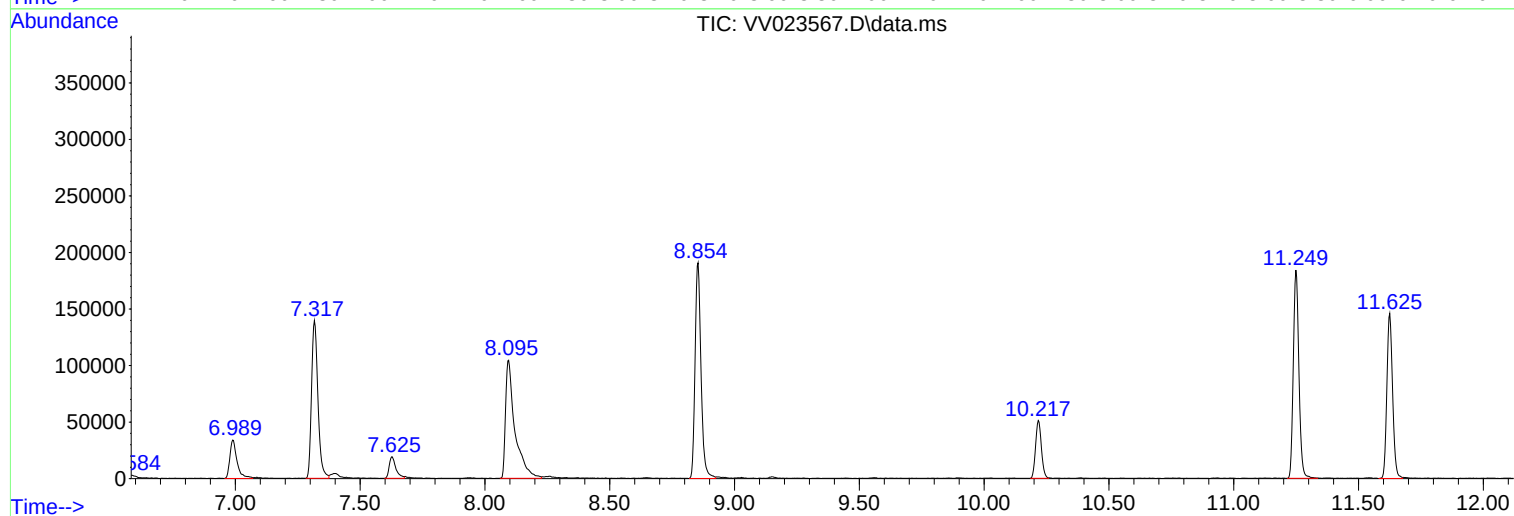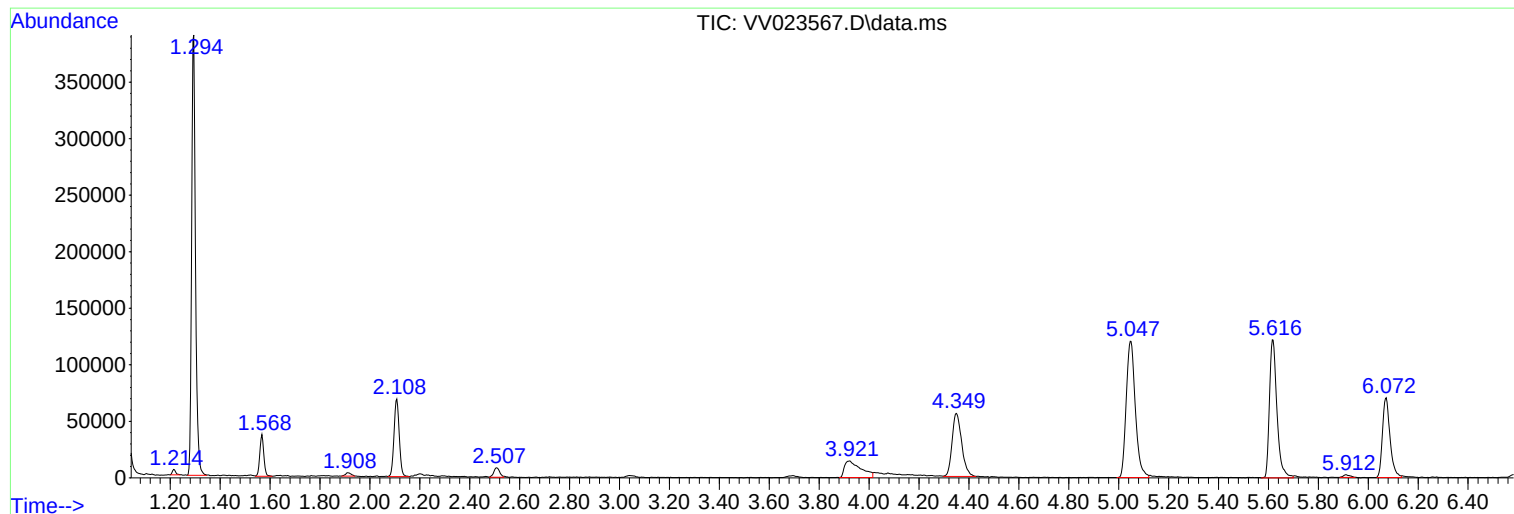

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023567.D
Acq On : 17 Nov 2021 14:13
Operator : SY/MD
Sample : M4643-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023567.D
Acq On : 17 Nov 2021 14:13
Operator : SY/MD
Sample : M4643-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
GB8K1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc