

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
 Data File : VV023570.D
 Acq On : 17 Nov 2021 15:24
 Operator : SY/MD
 Sample : M4616-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1Y7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023570.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	58	rBV	14341	12616	1.87%	0.330%
2	1.304	75	82	95	rVB	69428	71802	10.62%	1.876%
3	1.568	156	164	173	rBV	54036	59879	8.85%	1.565%
4	2.108	320	332	347	rBV	107697	157263	23.25%	4.110%
5	3.892	877	887	923	rBV3	33580	125736	18.59%	3.286%
6	4.349	1012	1029	1061	rBV	67472	171171	25.31%	4.473%
7	5.050	1229	1247	1273	rBV2	147184	368101	54.43%	9.620%
8	5.619	1412	1424	1449	rBV	120702	249860	36.94%	6.530%
9	5.915	1501	1516	1537	rBV	342162	676317	100.00%	17.674%
10	6.069	1553	1564	1585	rBV	80515	164096	24.26%	4.288%
11	6.989	1840	1850	1874	rBV	38675	74689	11.04%	1.952%
12	7.317	1940	1952	1973	rBV	178087	313631	46.37%	8.196%
13	7.625	2038	2048	2062	rBV	23404	41988	6.21%	1.097%
14	7.976	2146	2157	2180	rVB2	77186	134123	19.83%	3.505%
15	8.092	2182	2193	2222	rBV	129557	255464	37.77%	6.676%
16	8.854	2419	2430	2451	rBV	188691	312439	46.20%	8.165%
17	10.217	2843	2854	2868	rBV2	51917	81729	12.08%	2.136%
18	11.249	3165	3175	3194	rBV	182825	283574	41.93%	7.411%
19	11.532	3252	3263	3281	rBV3	8115	14963	2.21%	0.391%
20	11.625	3281	3292	3312	rVB	163131	257160	38.02%	6.720%




Sum of corrected areas: 3826601

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023570.D
Acq On : 17 Nov 2021 15:24
Operator : SY/MD
Sample : M4616-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

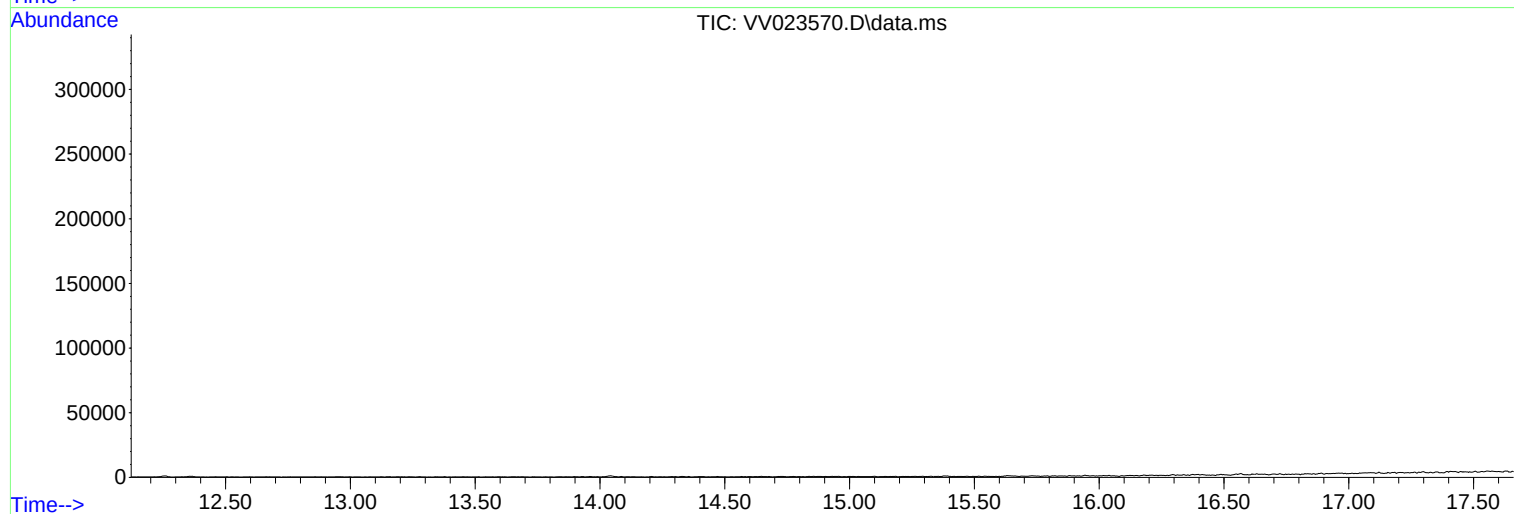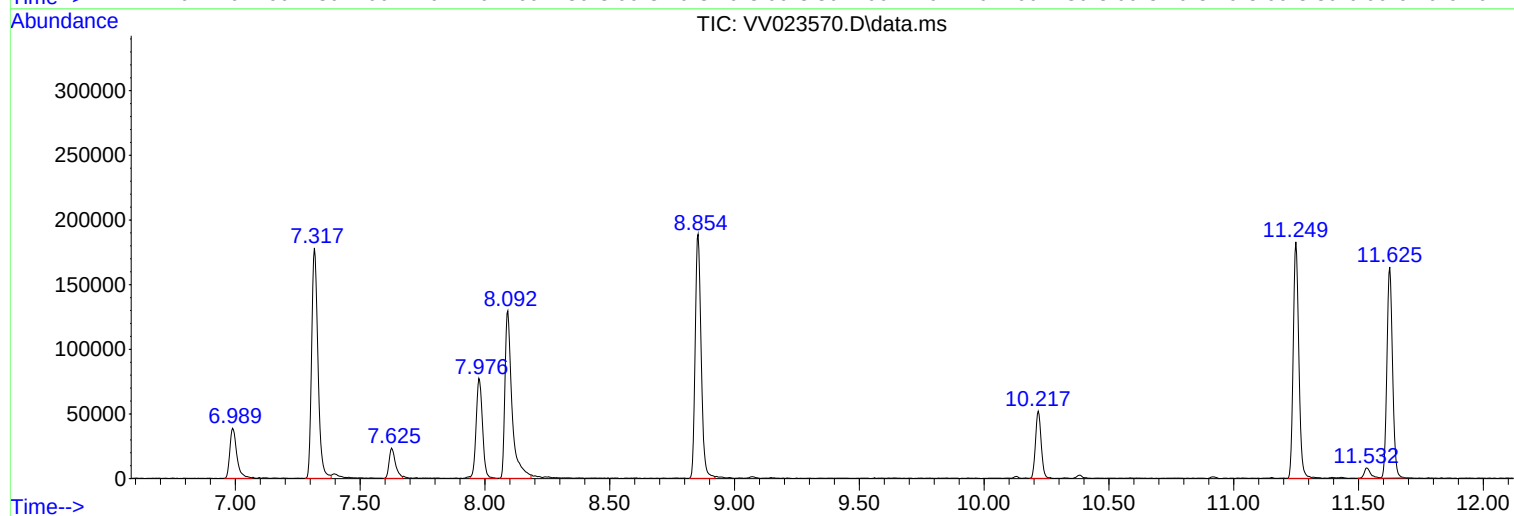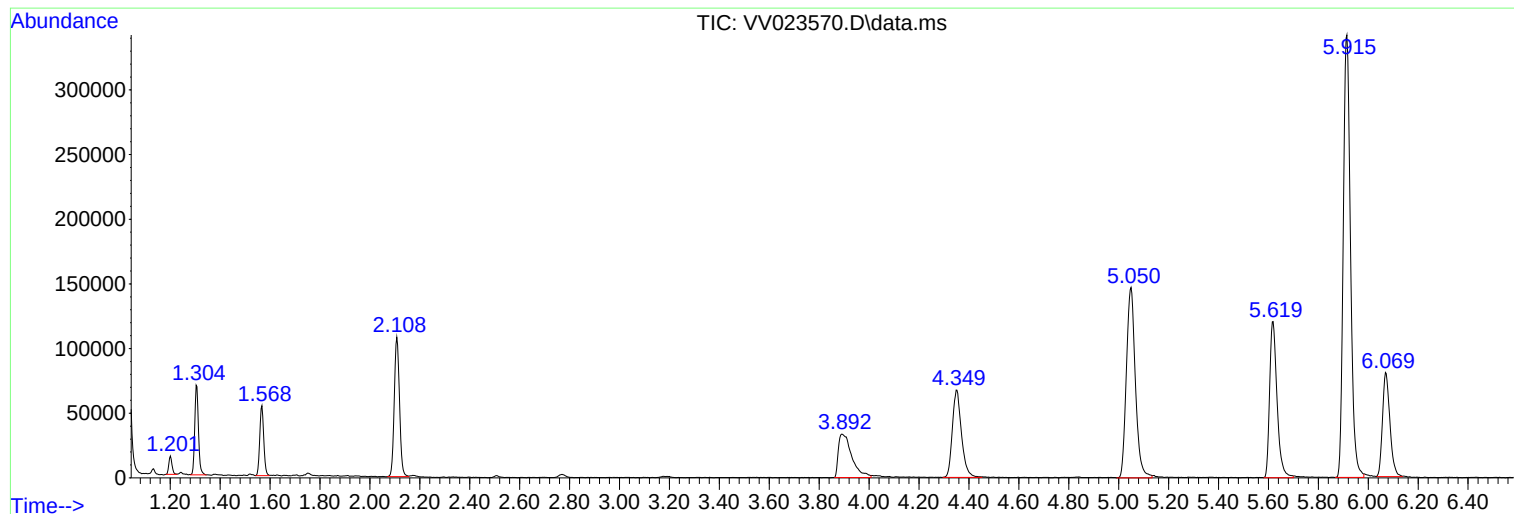

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023570.D
Acq On : 17 Nov 2021 15:24
Operator : SY/MD
Sample : M4616-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023570.D
Acq On : 17 Nov 2021 15:24
Operator : SY/MD
Sample : M4616-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc