

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
 Data File : VV023572.D
 Acq On : 17 Nov 2021 16:11
 Operator : SY/MD
 Sample : M4616-13DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BG1Y6DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV023572.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.201	44	50	59	rBV	95452	83578	22.09%	2.194%
2	1.307	72	83	94	rBV	67315	71832	18.99%	1.886%
3	1.568	157	164	176	rBV	55794	61373	16.22%	1.611%
4	2.108	321	332	346	rBV	109299	157115	41.53%	4.125%
5	2.510	448	457	469	rVB	7939	13879	3.67%	0.364%
6	3.905	876	891	920	rBV4	39213	146599	38.75%	3.849%
7	4.352	1015	1030	1054	rBV	65114	162945	43.08%	4.278%
8	5.050	1231	1247	1273	rBV2	149977	372037	98.35%	9.769%
9	5.619	1412	1424	1453	rBV	129525	265381	70.15%	6.968%
10	5.915	1504	1516	1540	rBV	127385	260644	68.90%	6.844%
11	6.072	1550	1565	1589	rBV2	81200	170445	45.06%	4.475%
12	6.989	1840	1850	1878	rBV	38881	75442	19.94%	1.981%
13	7.317	1941	1952	1970	rBV	181847	315188	83.32%	8.276%
14	7.625	2036	2048	2063	rBV	23810	42364	11.20%	1.112%
15	7.976	2136	2157	2180	rBV	218234	378279	100.00%	9.932%
16	8.091	2184	2193	2228	rBV	130241	257618	68.10%	6.764%
17	8.853	2419	2430	2453	rBV	197630	329407	87.08%	8.649%
18	10.217	2841	2854	2869	rBV2	52340	82953	21.93%	2.178%
19	10.384	2897	2906	2916	rVB5	5122	7894	2.09%	0.207%
20	11.249	3164	3175	3200	rBV	189956	297933	78.76%	7.823%
21	11.625	3281	3292	3309	rBV	161543	255630	67.58%	6.712%


Sum of corrected areas: 3808536

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023572.D
Acq On : 17 Nov 2021 16:11
Operator : SY/MD
Sample : M4616-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

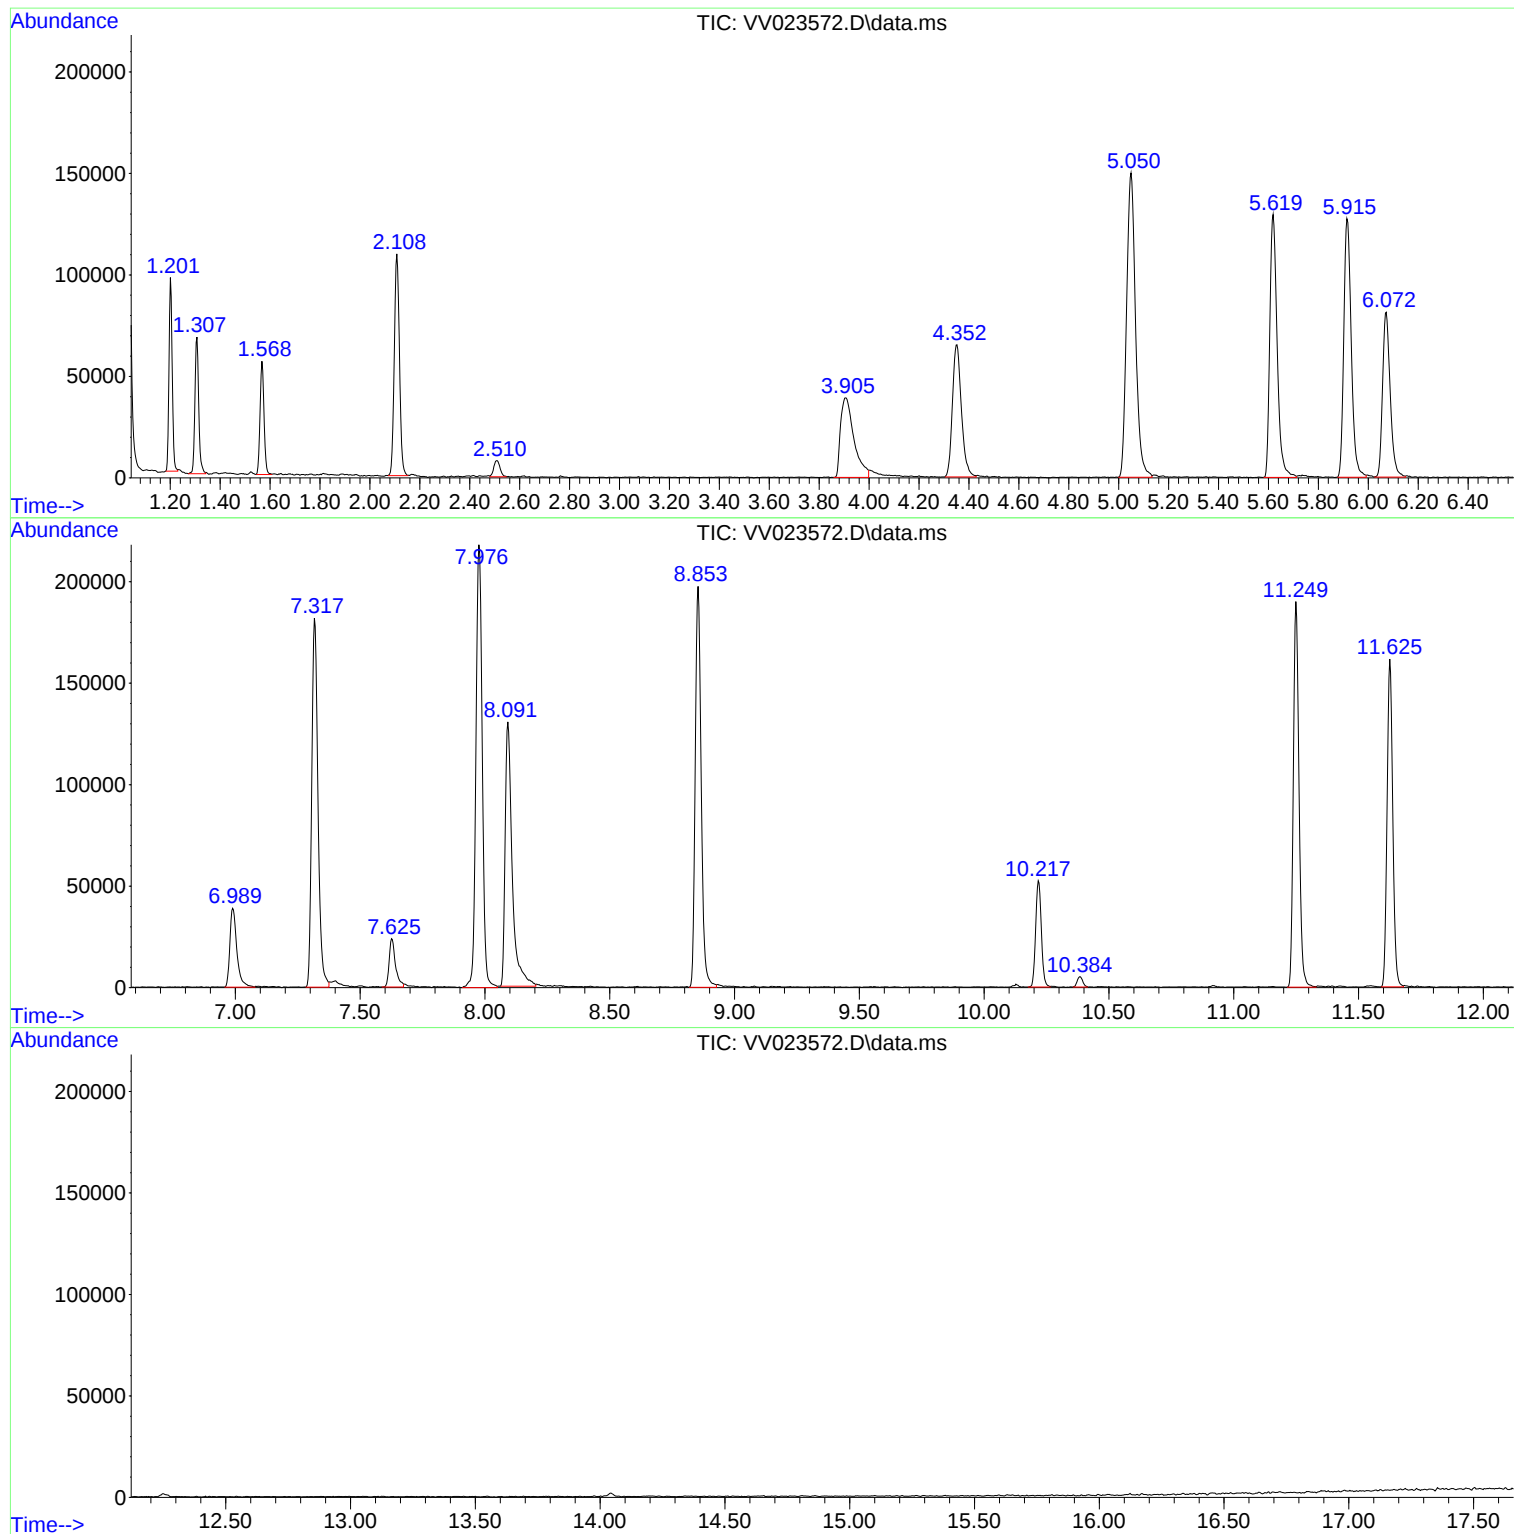

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023572.D
Acq On : 17 Nov 2021 16:11
Operator : SY/MD
Sample : M4616-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y6DL










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.201	1.57 ug/L	83578	1,4-Difluorobenzene	5.619

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Methyl nitrite	61	CH3NO2	000624-91-9	5
2			o-Ethylhydroxylamine	61	C2H7NO	000624-86-2	4
3			Methanamine, N-methoxy-	61	C2H7NO	001117-97-1	4
4			Carbonyl sulfide	60	COS	000463-58-1	4
5			Cyanogen chloride	61	CClN	000506-77-4	4

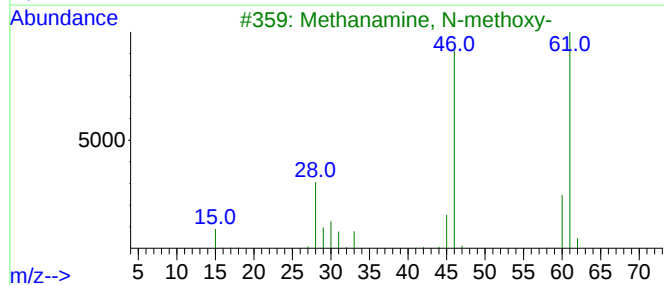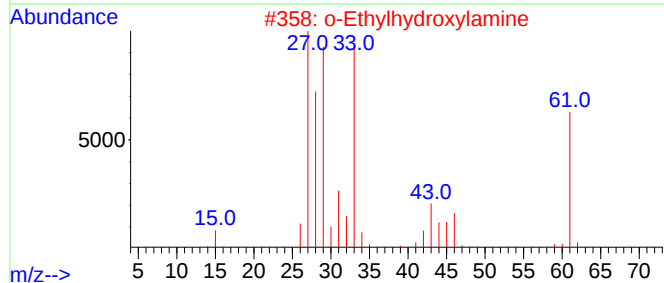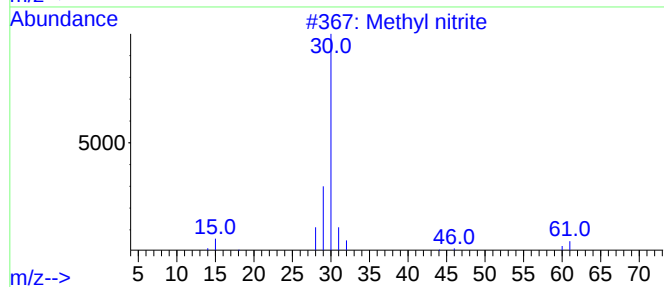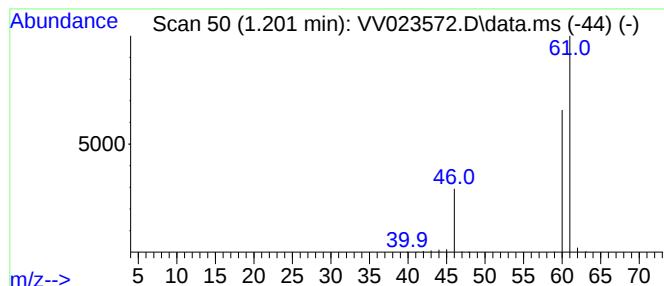

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023572.D
Acq On : 17 Nov 2021 16:11
Operator : SY/MD
Sample : M4616-13DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BG1Y6DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.201	1.6	ug/L	83578	1	5.619	265381	5.0