

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
 Data File : VV023578.D
 Acq On : 17 Nov 2021 18:35
 Operator : SY/MD
 Sample : M4627-01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H4630

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV023578.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	75	82	96	rVB	66904	66949	18.70%	2.269%
2	1.564	156	163	175	rVB	50228	56603	15.81%	1.919%
3	2.105	322	331	344	rBV	106677	150447	42.03%	5.100%
4	3.918	878	895	912	rBV2	13609	47854	13.37%	1.622%
5	4.352	1014	1030	1059	rVB4	57452	155985	43.58%	5.287%
6	5.050	1231	1247	1283	rBV2	143793	355899	99.43%	12.064%
7	5.619	1412	1424	1448	rBV	141638	286380	80.01%	9.708%
8	5.918	1506	1517	1532	rVB6	2830	6561	1.83%	0.222%
9	6.072	1551	1565	1592	rBV	77165	163505	45.68%	5.542%
10	6.989	1840	1850	1866	rBV	35927	68494	19.14%	2.322%
11	7.317	1941	1952	1970	rBV	167924	293649	82.04%	9.954%
12	7.400	1974	1978	1991	rVB3	3250	5193	1.45%	0.176%
13	7.625	2039	2048	2066	rBV2	20076	39188	10.95%	1.328%
14	8.095	2182	2194	2230	rBV2	93797	249689	69.76%	8.464%
15	8.853	2419	2430	2456	rBV	221959	357941	100.00%	12.133%
16	10.217	2843	2854	2867	rBV2	50454	79184	22.12%	2.684%
17	11.249	3165	3175	3197	rBV	200159	314841	87.96%	10.672%
18	11.625	3280	3292	3307	rBV	156106	243512	68.03%	8.254%
19	14.040	4035	4043	4058	rVB2	5522	8214	2.29%	0.278%




Sum of corrected areas: 2950088

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023578.D
Acq On : 17 Nov 2021 18:35
Operator : SY/MD
Sample : M4627-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4630

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

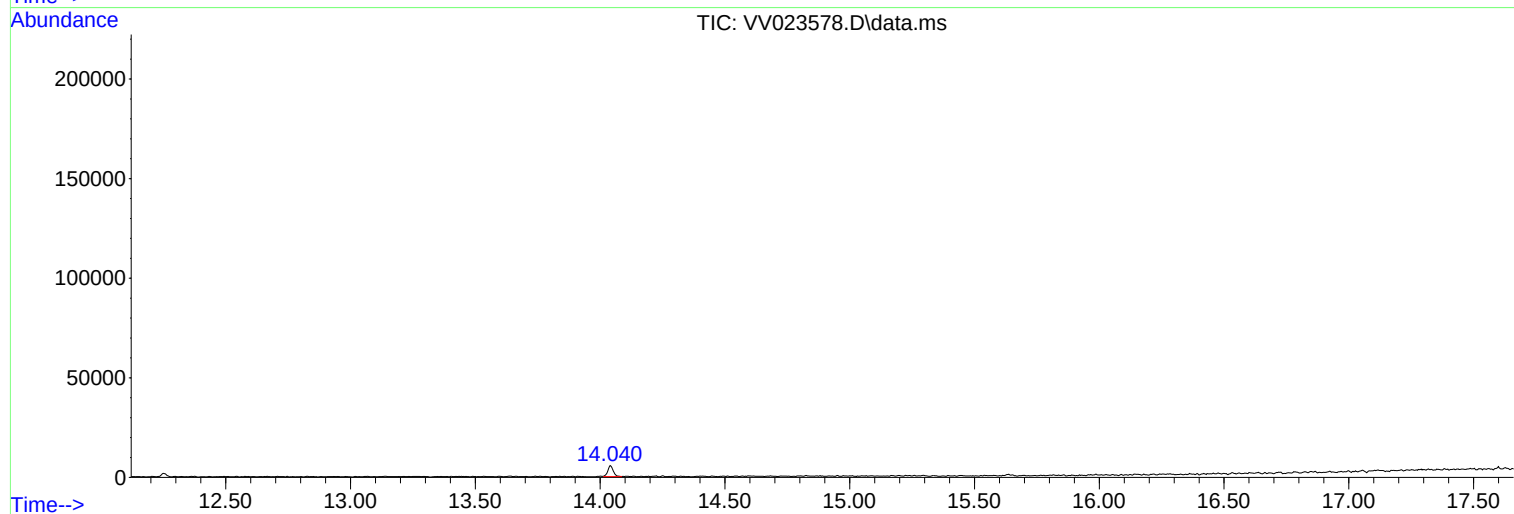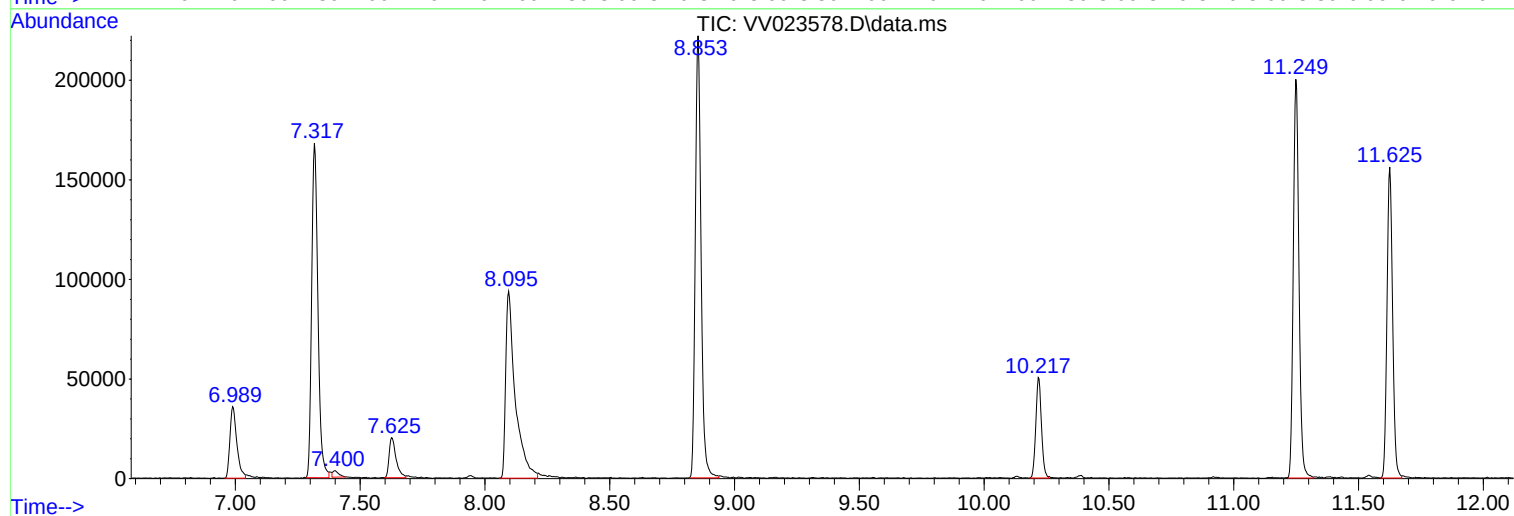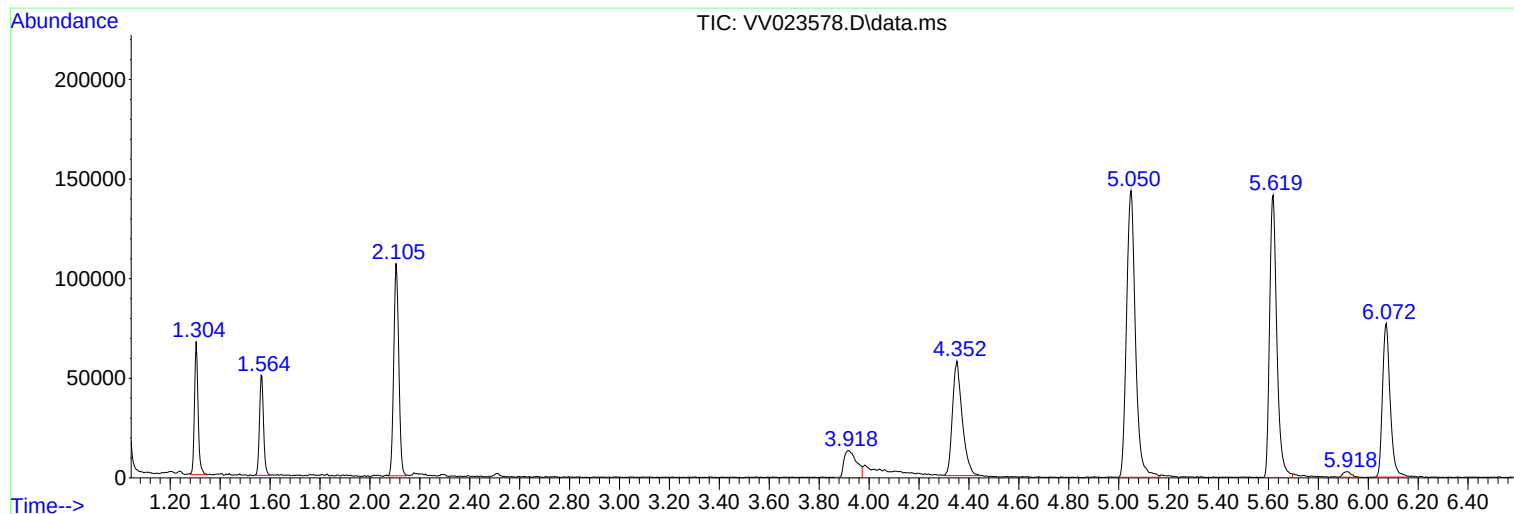

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023578.D
Acq On : 17 Nov 2021 18:35
Operator : SY/MD
Sample : M4627-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4630

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
Data File : VV023578.D
Acq On : 17 Nov 2021 18:35
Operator : SY/MD
Sample : M4627-01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H4630

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc