


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111721\
 Data File : VV023564.D
 Acq On : 17 Nov 2021 12:22
 Operator : SY/MD
 Sample : BFB236
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB236

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR110421WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Thu Nov 18 00:20:29 2021

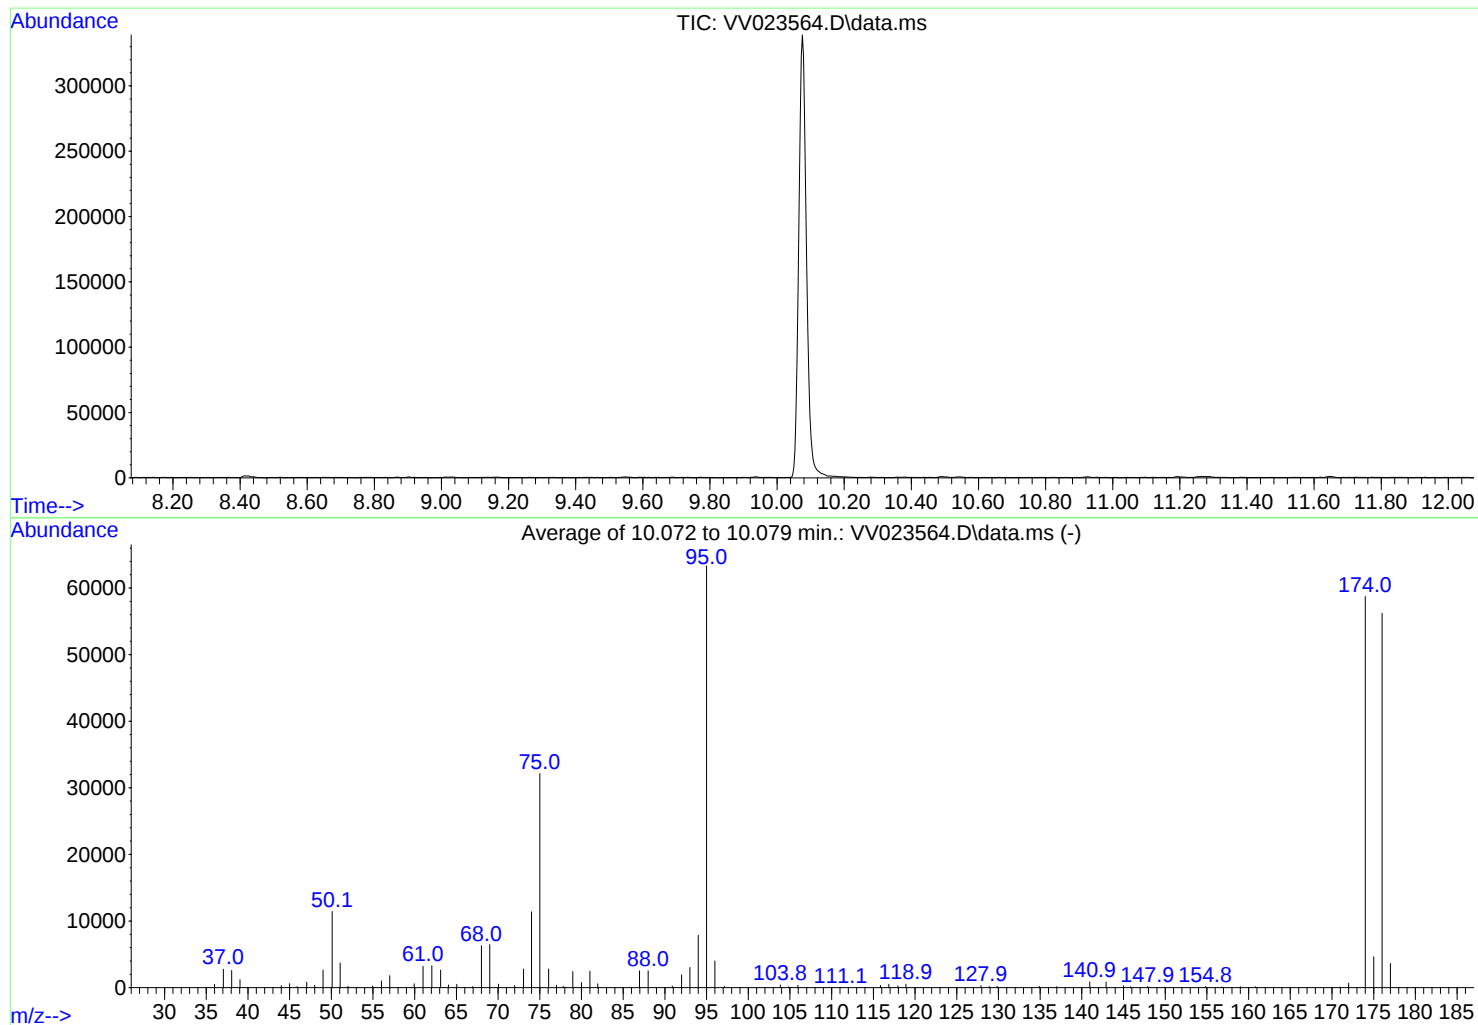

AutoFind: Scans 2809, 2810, 2811; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	11442	PASS
75	95	30	80	50.8	32149	PASS
95	95	100	100	100.0	63331	PASS
96	95	5	9	6.3	4008	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	92.7	58725	PASS
175	174	5	9	7.9	4646	PASS
176	174	95	105	95.7	56224	PASS
177	176	5	10	6.5	3636	PASS

m/z	Abundance
39.90	170.0
44.10	194.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
36.00	502.0
37.10	2789.0
38.00	2686.0
39.00	1200.0
40.00	174.0
44.00	489.0
45.00	626.0
45.90	191.0
47.00	754.0
48.00	296.0
49.00	2690.0
50.10	11511.0
51.10	3693.0
52.00	281.0
53.10	136.0
55.00	235.0
56.00	980.0
57.00	1808.0
60.00	557.0
61.00	3318.0
62.00	3444.0
63.10	2664.0
64.10	460.0
65.00	517.0
67.00	177.0
68.00	6218.0
69.00	6589.0
70.00	519.0
72.00	357.0
73.00	2728.0
74.00	11354.0
75.00	32408.0
76.00	2822.0
77.00	366.0
77.80	341.0
78.90	2359.0
80.00	835.0
81.00	2420.0
82.00	623.0
85.90	137.0
86.90	2479.0
88.00	2561.0
90.90	244.0
92.00	1914.0
93.00	2877.0
94.00	7717.0
95.00	62680.0
96.00	4048.0
97.10	159.0
103.80	382.0
104.80	168.0
105.90	392.0
111.10	103.0
115.80	366.0
116.80	486.0
117.90	238.0
118.90	562.0
128.00	318.0
128.90	170.0
129.80	216.0
134.90	204.0
136.90	166.0
140.90	858.0
142.90	842.0
145.00	193.0
145.80	144.0
147.90	145.0
152.00	114.0
154.90	143.0
156.80	129.0
159.00	129.0
160.90	189.0
171.00	167.0
172.00	676.0
174.00	56488.0
175.00	4552.0
176.00	53464.0
177.00	3497.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
36.00	529.0
37.10	2833.0
38.00	2640.0
39.00	1245.0
39.90	157.0
44.00	518.0
45.00	614.0
45.90	199.0
47.10	847.0
48.00	375.0
49.00	2727.0
50.10	11848.0
51.10	3821.0
52.00	232.0
53.10	108.0
54.90	244.0
56.00	1047.0
57.00	1895.0
59.90	599.0
61.00	3298.0
62.00	3393.0
63.10	2744.0
64.10	411.0
65.00	517.0
66.00	111.0
66.90	137.0
68.00	6561.0
69.00	6689.0
70.10	548.0
71.10	121.0
72.00	336.0
73.00	2875.0
74.00	11693.0
75.00	33144.0
76.10	2894.0
77.00	367.0
77.80	297.0
79.00	2498.0
80.00	801.0
81.00	2540.0
81.90	603.0
85.90	117.0
86.90	2654.0
88.00	2631.0
90.90	267.0
92.00	2009.0
93.00	3142.0
94.00	8136.0
95.00	65544.0
96.00	4148.0
97.20	172.0
103.80	404.0
104.80	160.0
106.00	384.0
115.80	357.0
116.90	533.0
117.90	284.0
118.90	577.0
127.90	323.0
128.90	197.0
129.80	222.0
134.90	193.0
136.90	158.0
141.00	905.0
142.90	907.0
145.00	297.0
145.80	140.0
147.90	177.0
149.90	118.0
154.90	165.0
156.80	125.0
159.00	152.0
160.80	172.0
170.90	142.0
172.00	679.0
174.00	60744.0
175.00	4756.0
176.00	57984.0
177.00	3802.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236

m/z	Abundance
36.00	515.0
37.00	2648.0
38.10	2367.0
39.10	1134.0
40.00	120.0
44.00	492.0
45.00	566.0
45.90	152.0
47.10	831.0
48.00	430.0
49.00	2541.0
50.10	10966.0
51.00	3563.0
52.00	165.0
54.90	244.0
56.00	1031.0
57.00	1733.0
59.90	598.0
61.00	2986.0
62.10	3031.0
63.10	2558.0
63.90	388.0
65.10	476.0
66.90	119.0
68.00	6088.0
69.00	6124.0
70.10	551.0
71.00	106.0
72.00	324.0
73.10	2787.0
74.00	11089.0
75.00	30896.0
76.10	2742.0
77.00	392.0
78.10	237.0
79.00	2382.0
80.00	688.0
81.00	2454.0
81.90	546.0
87.00	2406.0
88.00	2431.0
90.90	255.0
92.00	1881.0
93.00	3033.0
94.00	7729.0
95.00	61768.0
96.00	3829.0
97.20	172.0
103.90	416.0
104.80	145.0
106.00	326.0
115.90	272.0
116.90	534.0
118.00	290.0
118.90	464.0
127.80	314.0
128.90	179.0
129.90	246.0
134.90	159.0
137.00	139.0
141.00	840.0
142.20	131.0
142.90	809.0
143.90	125.0
145.00	338.0
145.90	128.0
147.90	239.0
149.90	138.0
154.00	107.0
154.80	178.0
156.80	136.0
159.00	149.0
160.80	113.0
170.20	101.0
172.00	659.0
174.00	58944.0
175.00	4630.0
176.00	57224.0
177.00	3608.0

Instrument :
MSVOA_V
ClientSampleId :
BFB236