




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
 Data File : VV029058.D
 Acq On : 17 Nov 2022 13:04
 Operator : SY/MD
 Sample : N5621-02DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCB9DL

Manual IntegrationsAPPROVED

Quant Time: Nov 18 01:41:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 01:37:41 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/18/2022
 Supervised By :Mahesh Dadoda 11/18/2022

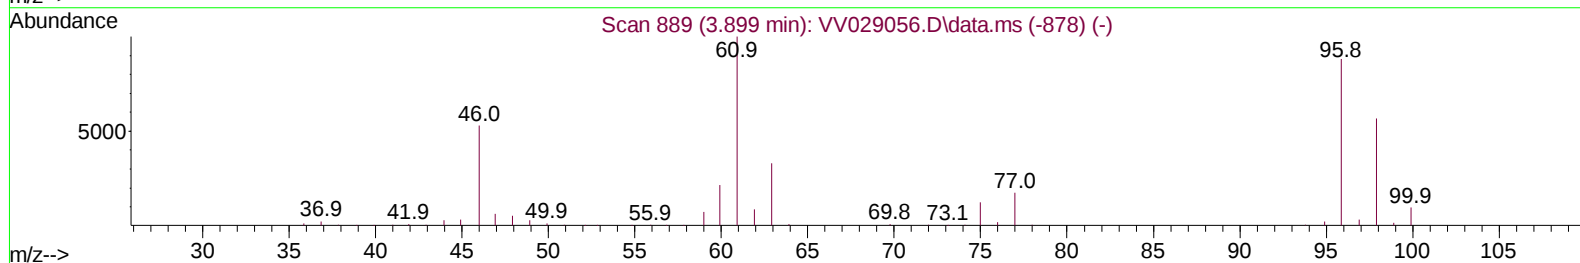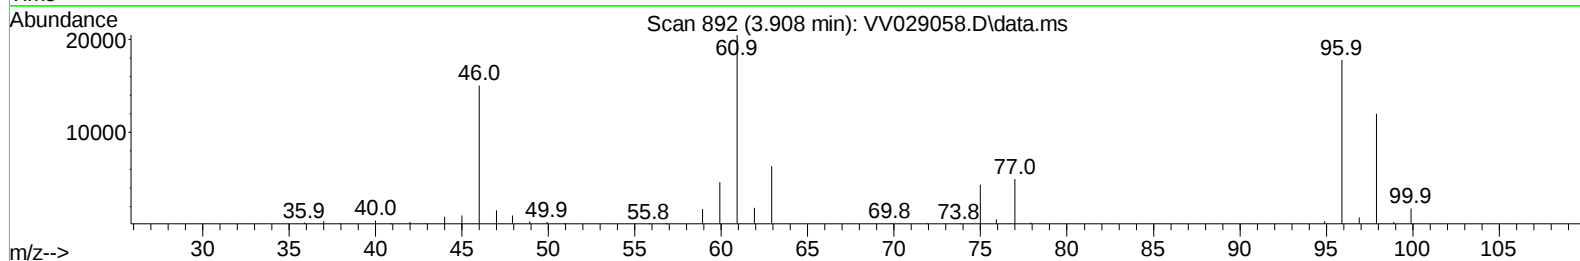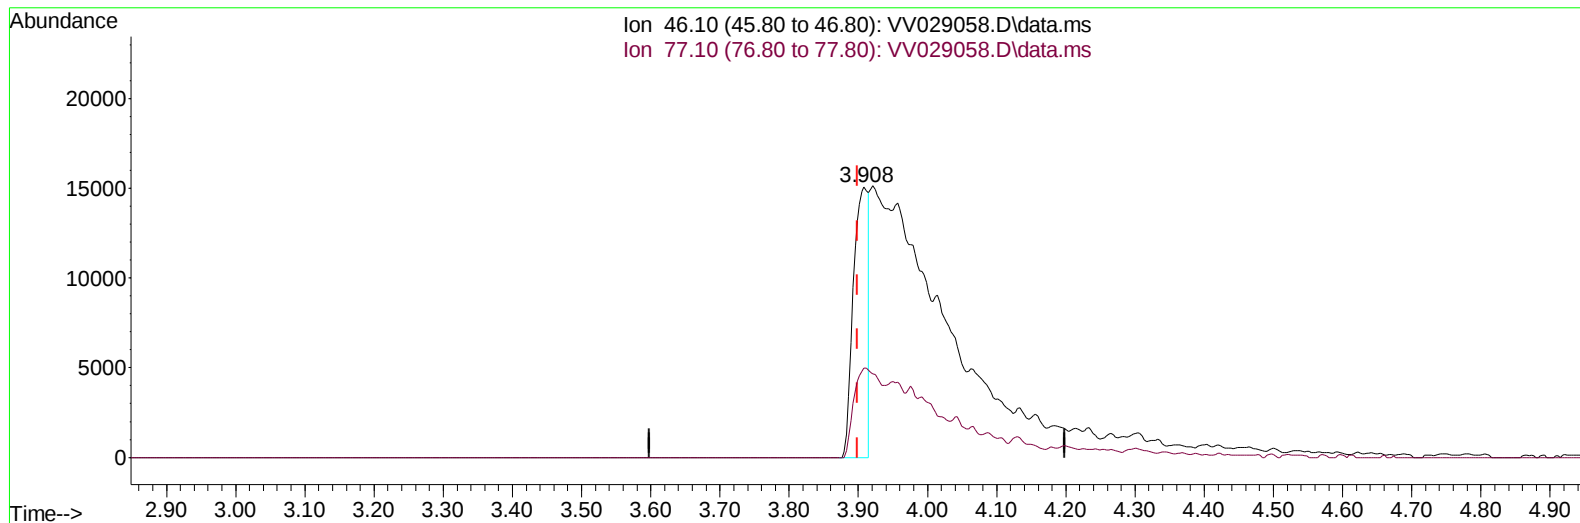

TIC: VV029058.D\data.ms

(20) 2-Butanone-d5 (S)

3.908min (+ 0.010) 9.09 ug/L

response 23047

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.70	61.48#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029058.D
Acq On : 17 Nov 2022 13:04
Operator : SY/MD
Sample : N5621-02DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB9DL

Manual IntegrationsAPPROVED

Quant Time: Nov 18 01:41:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 01:37:41 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/18/2022
Supervised By :Mahesh Dadoda 11/18/2022

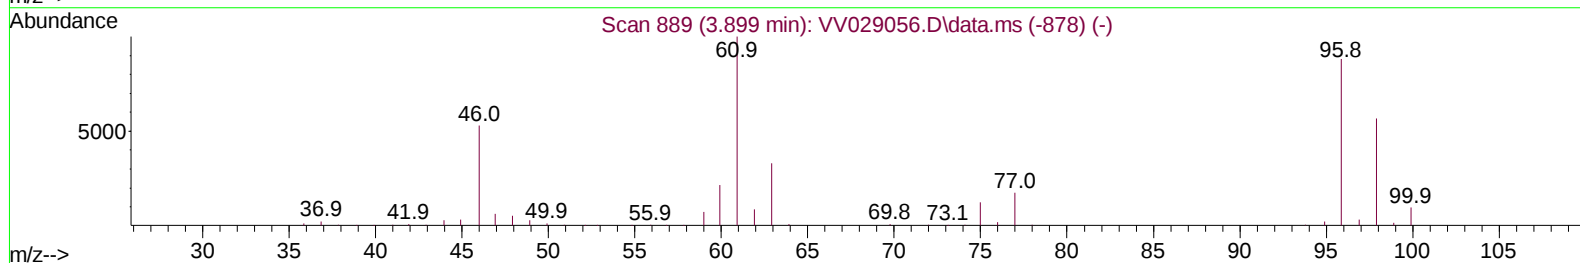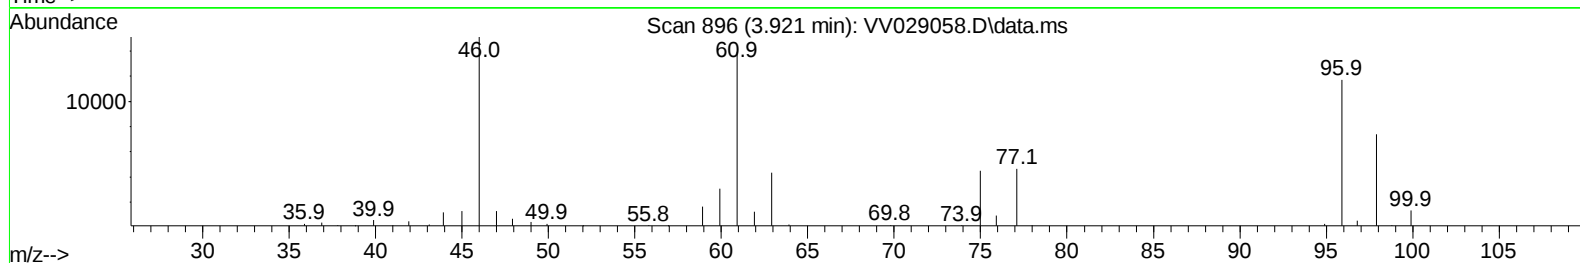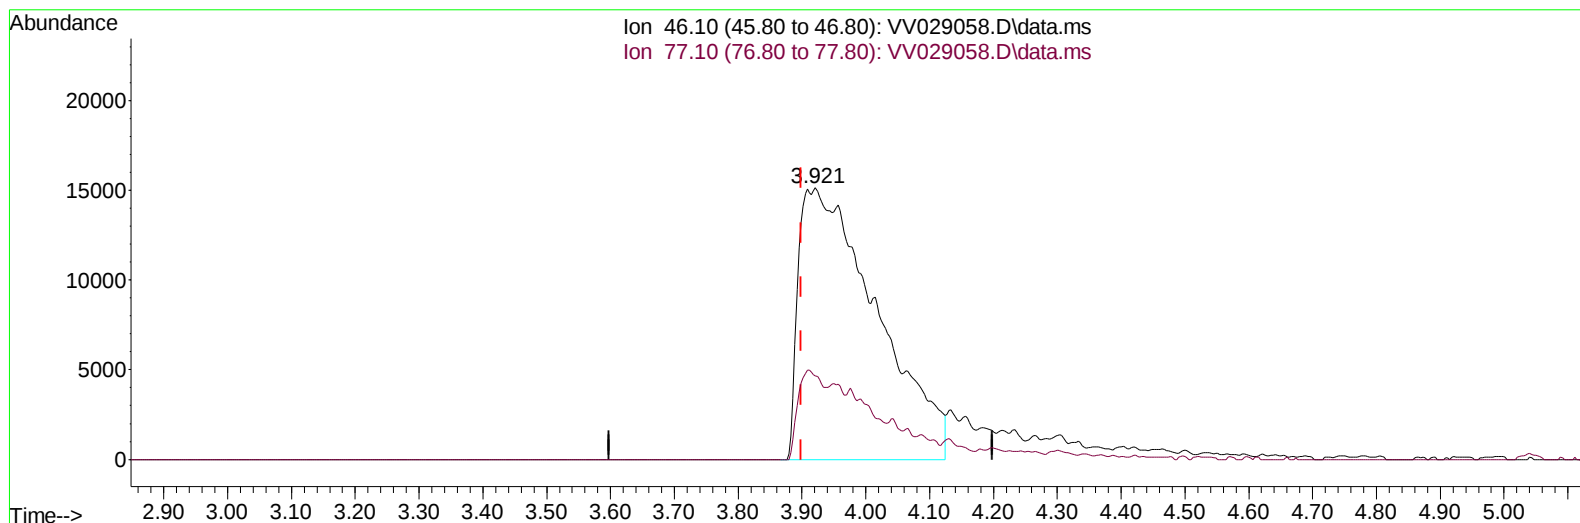

TIC: VV029058.D\data.ms

(20) 2-Butanone-d5 (S)

3.921min (+ 0.023) 50.57 ug/L m

response 128192

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.70	11.05#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
 Data File : VV029058.D
 Acq On : 17 Nov 2022 13:04
 Operator : SY/MD
 Sample : N5621-02DL 5X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCB9DL

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/18/2022
 Supervised By :Mahesh Dadoda 11/18/2022

Quant Time: Nov 18 01:41:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 01:37:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	248379	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	229256	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	109037	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	62869	4.152	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	83.000%	
7) Chloroethane-d5	1.564	69	54402	4.087	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130	Recovery	=	81.800%	
11) 1,1-Dichloroethene-d2	2.101	63	89371	3.239	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	64.800%	
20) 2-Butanone-d5	3.921	46	128192m	50.573	ug/L	0.02
Spiked Amount 50.000	Range 40	- 130	Recovery	=	101.140%	
24) Chloroform-d	4.339	84	153031	4.922	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	98.400%	
26) 1,2-Dichloroethane-d4	5.027	65	71020	5.077	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	101.600%	
32) Benzene-d6	5.043	84	322218	4.709	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	94.200%	
36) 1,2-Dichloropropane-d6	6.063	67	92870	4.860	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140	Recovery	=	97.200%	
41) Toluene-d8	7.310	98	292843	4.754	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130	Recovery	=	95.000%	
43) trans-1,3-Dichloroprop...	7.622	79	32403	5.199	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130	Recovery	=	104.000%	
46) 2-Hexanone-d5	8.088	63	123998	46.613	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130	Recovery	=	93.220%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	67101	5.065	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	101.200%	
66) 1,2-Dichlorobenzene-d4	11.615	152	110431	5.661	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	113.200%	
Target Compounds						
16) Methylene chloride	2.503	84	20654	1.062	ug/L	93
19) 1,1-Dichloroethane	3.185	63	5306	0.186	ug/L	91
22) cis-1,2-Dichloroethene	3.905	96	43405	2.448	ug/L	99
34) Trichloroethene	5.908	95	123779	6.901	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029058.D
Acq On : 17 Nov 2022 13:04
Operator : SY/MD
Sample : N5621-02DL 5X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCB9DL

Manual IntegrationsAPPROVED

Quant Time: Nov 18 01:41:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 01:37:41 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/18/2022
Supervised By :Mahesh Dadoda 11/18/2022

