

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
 Data File : VV029062.D
 Acq On : 17 Nov 2022 14:39
 Operator : SY/MD
 Sample : N5592-20
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 18 01:42:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 01:37:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	255781	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	229680	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	109687	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	56793	3.642	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	72.800%	
7) Chloroethane-d5	1.561	69	51847	3.782	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	75.600%	
11) 1,1-Dichloroethene-d2	2.101	63	87081	3.064	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	61.200%	
20) 2-Butanone-d5	3.918	46	136658	52.353	ug/L	0.02
Spiked Amount	50.000	Range 40 - 130	Recovery	=	104.700%	
24) Chloroform-d	4.342	84	152069	4.750	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	95.000%	
26) 1,2-Dichloroethane-d4	5.030	65	72137	5.008	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	100.200%	
32) Benzene-d6	5.047	84	320233	4.671	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	93.400%	
36) 1,2-Dichloropropane-d6	6.066	67	91604	4.785	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	95.800%	
41) Toluene-d8	7.313	98	293049	4.749	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	95.000%	
43) trans-1,3-Dichloroprop...	7.622	79	30944	4.956	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	99.200%	
46) 2-Hexanone-d5	8.088	63	125987	47.273	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	94.540%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	68363	5.151	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	103.000%	
66) 1,2-Dichlorobenzene-d4	11.615	152	112004	5.707	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	114.200%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	8391	0.419	ug/L	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029062.D
Acq On : 17 Nov 2022 14:39
Operator : SY/MD
Sample : N5592-20
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Nov 18 01:42:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 01:37:41 2022
Response via : Initial Calibration

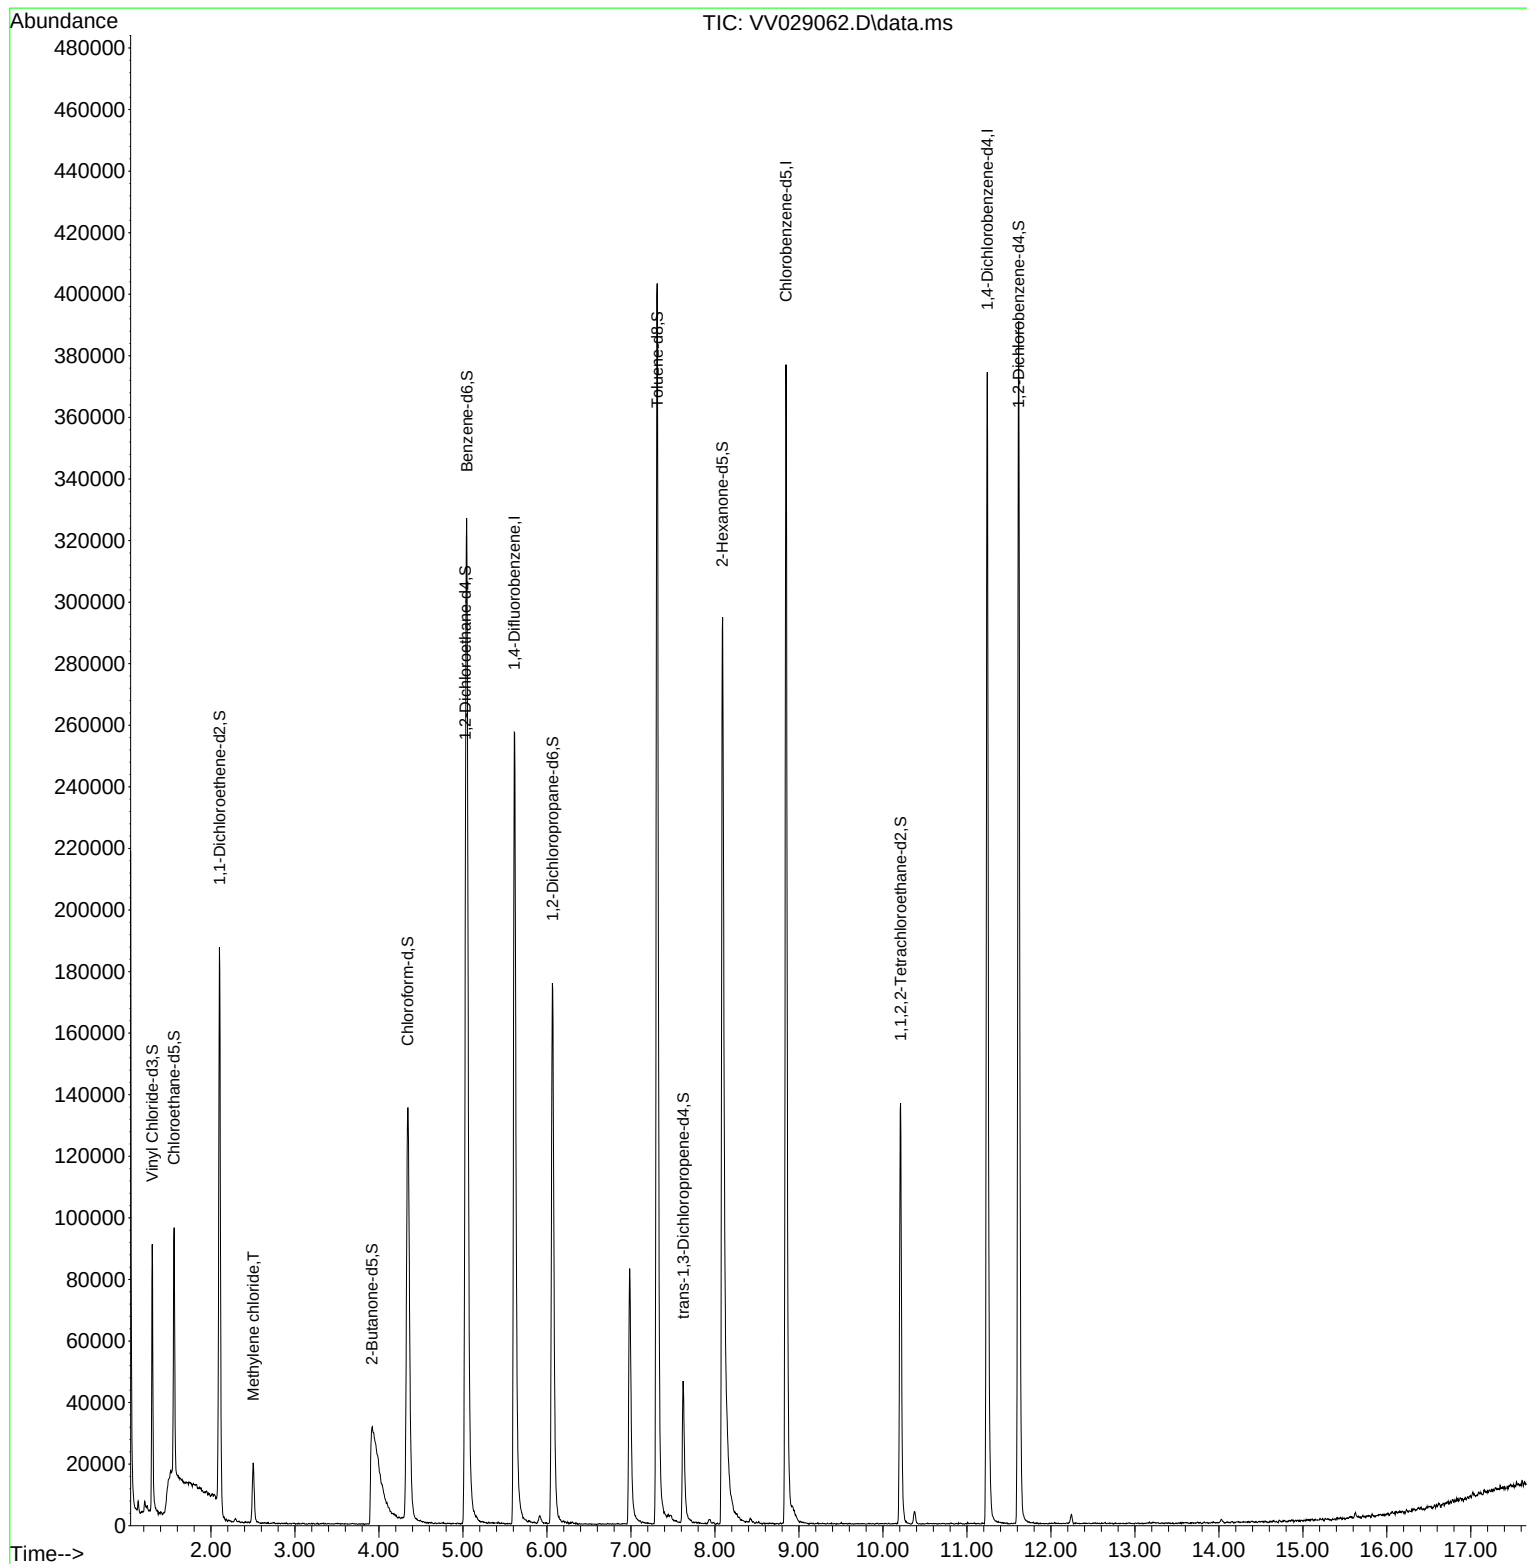

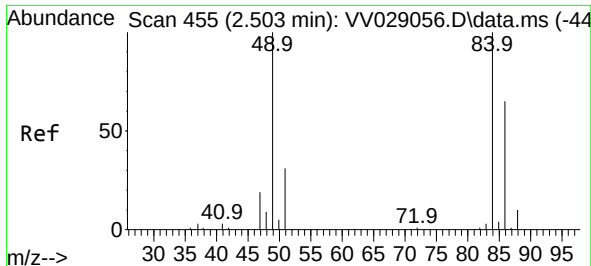

#16
Methylene chloride
Concen: 0.419 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.000 min
Lab File: VV029062.D
Acq: 17 Nov 2022 14:39

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion: 84 Resp: 8391
Ion Ratio Lower Upper
84 100
86 66.3 45.8 85.0
49 113.1 75.5 140.1

