

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
 Data File : VV029070.D
 Acq On : 17 Nov 2022 17:49
 Operator : SY/MD
 Sample : N5628-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 18 01:44:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 01:37:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	273149	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	249432	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	120067	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	61196	3.675	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	73.400%	
7) Chloroethane-d5	1.568	69	52200	3.566	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	71.400%	
11) 1,1-Dichloroethene-d2	2.105	63	87894	2.896	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	58.000%#	
20) 2-Butanone-d5	3.902	46	110473	39.631	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	79.260%	
24) Chloroform-d	4.342	84	149937	4.386	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	87.800%	
26) 1,2-Dichloroethane-d4	5.030	65	70576	4.588	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	91.800%	
32) Benzene-d6	5.047	84	313887	4.216	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	84.400%	
36) 1,2-Dichloropropane-d6	6.066	67	90360	4.346	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	87.000%	
41) Toluene-d8	7.310	98	292649	4.367	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	87.400%	
43) trans-1,3-Dichloroprop...	7.622	79	22918	3.380	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	67.600%	
46) 2-Hexanone-d5	8.088	63	120856	41.757	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	83.520%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	66737	4.630	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	92.600%	
66) 1,2-Dichlorobenzene-d4	11.615	152	109308	5.089	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	101.800%	
Target Compounds						Qvalue
16) Methylene chloride	2.506	84	9166	0.429	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029070.D
Acq On : 17 Nov 2022 17:49
Operator : SY/MD
Sample : N5628-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 18 01:44:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 01:37:41 2022
Response via : Initial Calibration

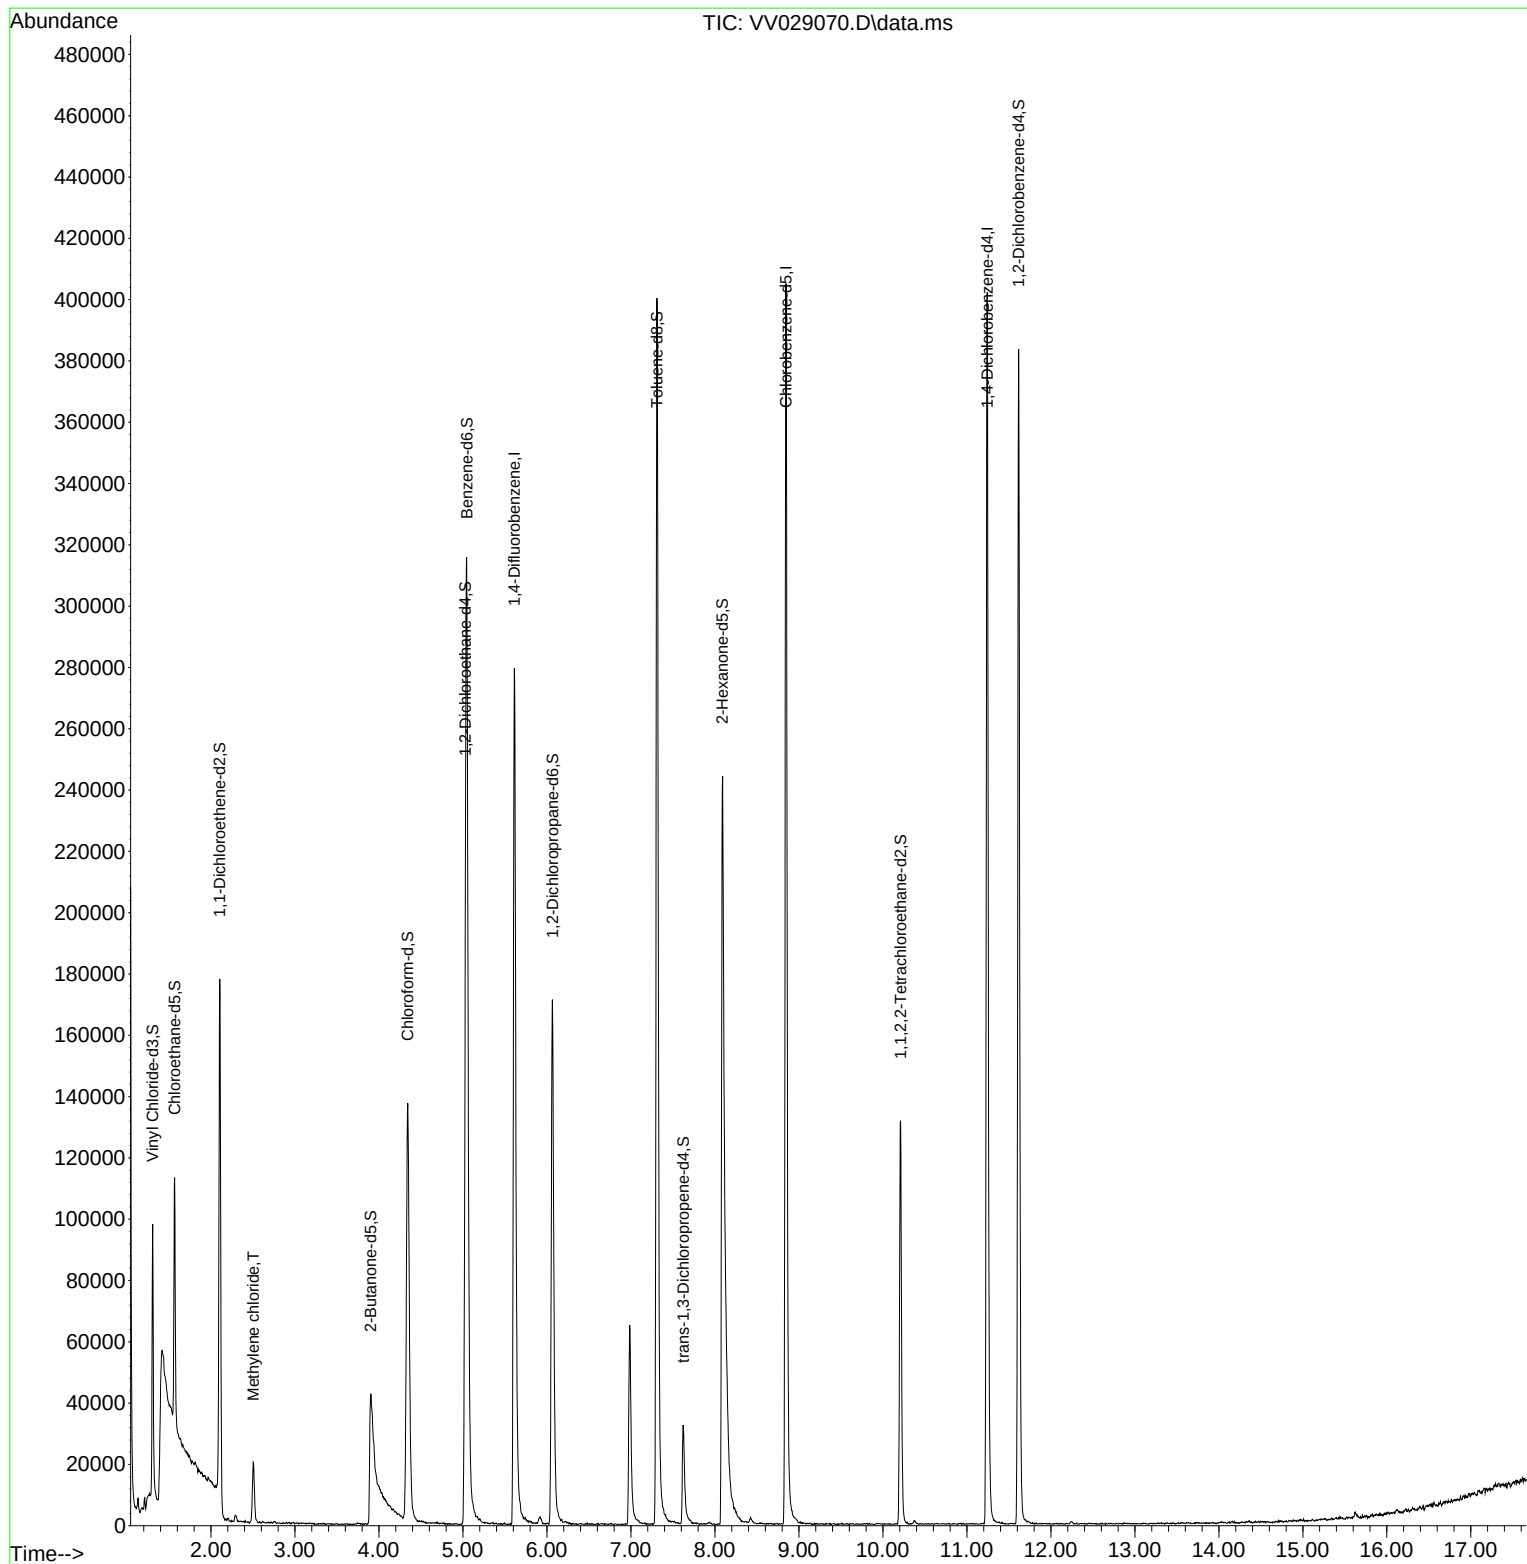

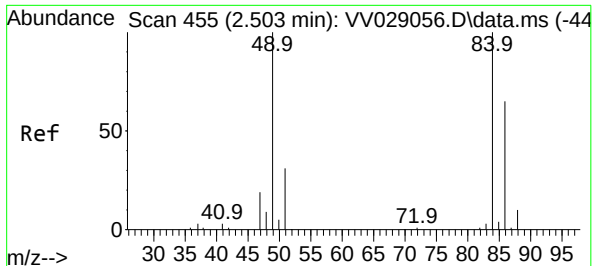

#16
Methylene chloride
Concen: 0.429 ug/L
RT: 2.506 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV029070.D
Acq: 17 Nov 2022 17:49

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

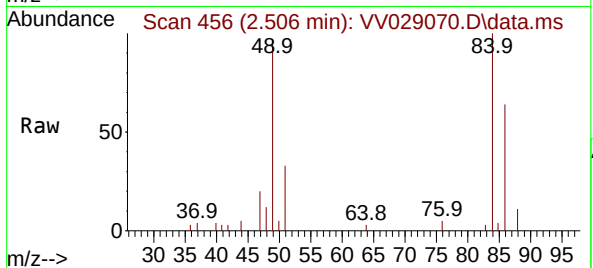

Tgt Ion: 84 Resp: 9166
Ion Ratio Lower Upper
84 100
86 64.4 45.8 85.0
49 97.0 75.5 140.1

