

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
 Data File : VV029074.D
 Acq On : 17 Nov 2022 19:25
 Operator : SY/MD
 Sample : N5620-21
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 18 01:44:58 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 01:37:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	263037	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	240614	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	110364	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	63156	3.938	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	78.800%
7) Chloroethane-d5	1.568	69	53070	3.765	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	75.200%
11) 1,1-Dichloroethene-d2	2.105	63	88346	3.023	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	60.400%
20) 2-Butanone-d5	3.899	46	142311	53.015	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.020%
24) Chloroform-d	4.346	84	152889	4.644	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.800%
26) 1,2-Dichloroethane-d4	5.031	65	72269	4.879	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.600%
32) Benzene-d6	5.047	84	313334	4.363	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	87.200%
36) 1,2-Dichloropropane-d6	6.066	67	92863	4.630	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	92.600%
41) Toluene-d8	7.314	98	289418	4.477	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	89.600%
43) trans-1,3-Dichloroprop...	7.622	79	24662	3.770	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	75.400%
46) 2-Hexanone-d5	8.088	63	123945	44.394	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.780%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	67224	4.835	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.600%
66) 1,2-Dichlorobenzene-d4	11.616	152	109295	5.535	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	110.800%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	6827	0.332	ug/L	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029074.D
Acq On : 17 Nov 2022 19:25
Operator : SY/MD
Sample : N5620-21
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 18 01:44:58 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 01:37:41 2022
Response via : Initial Calibration

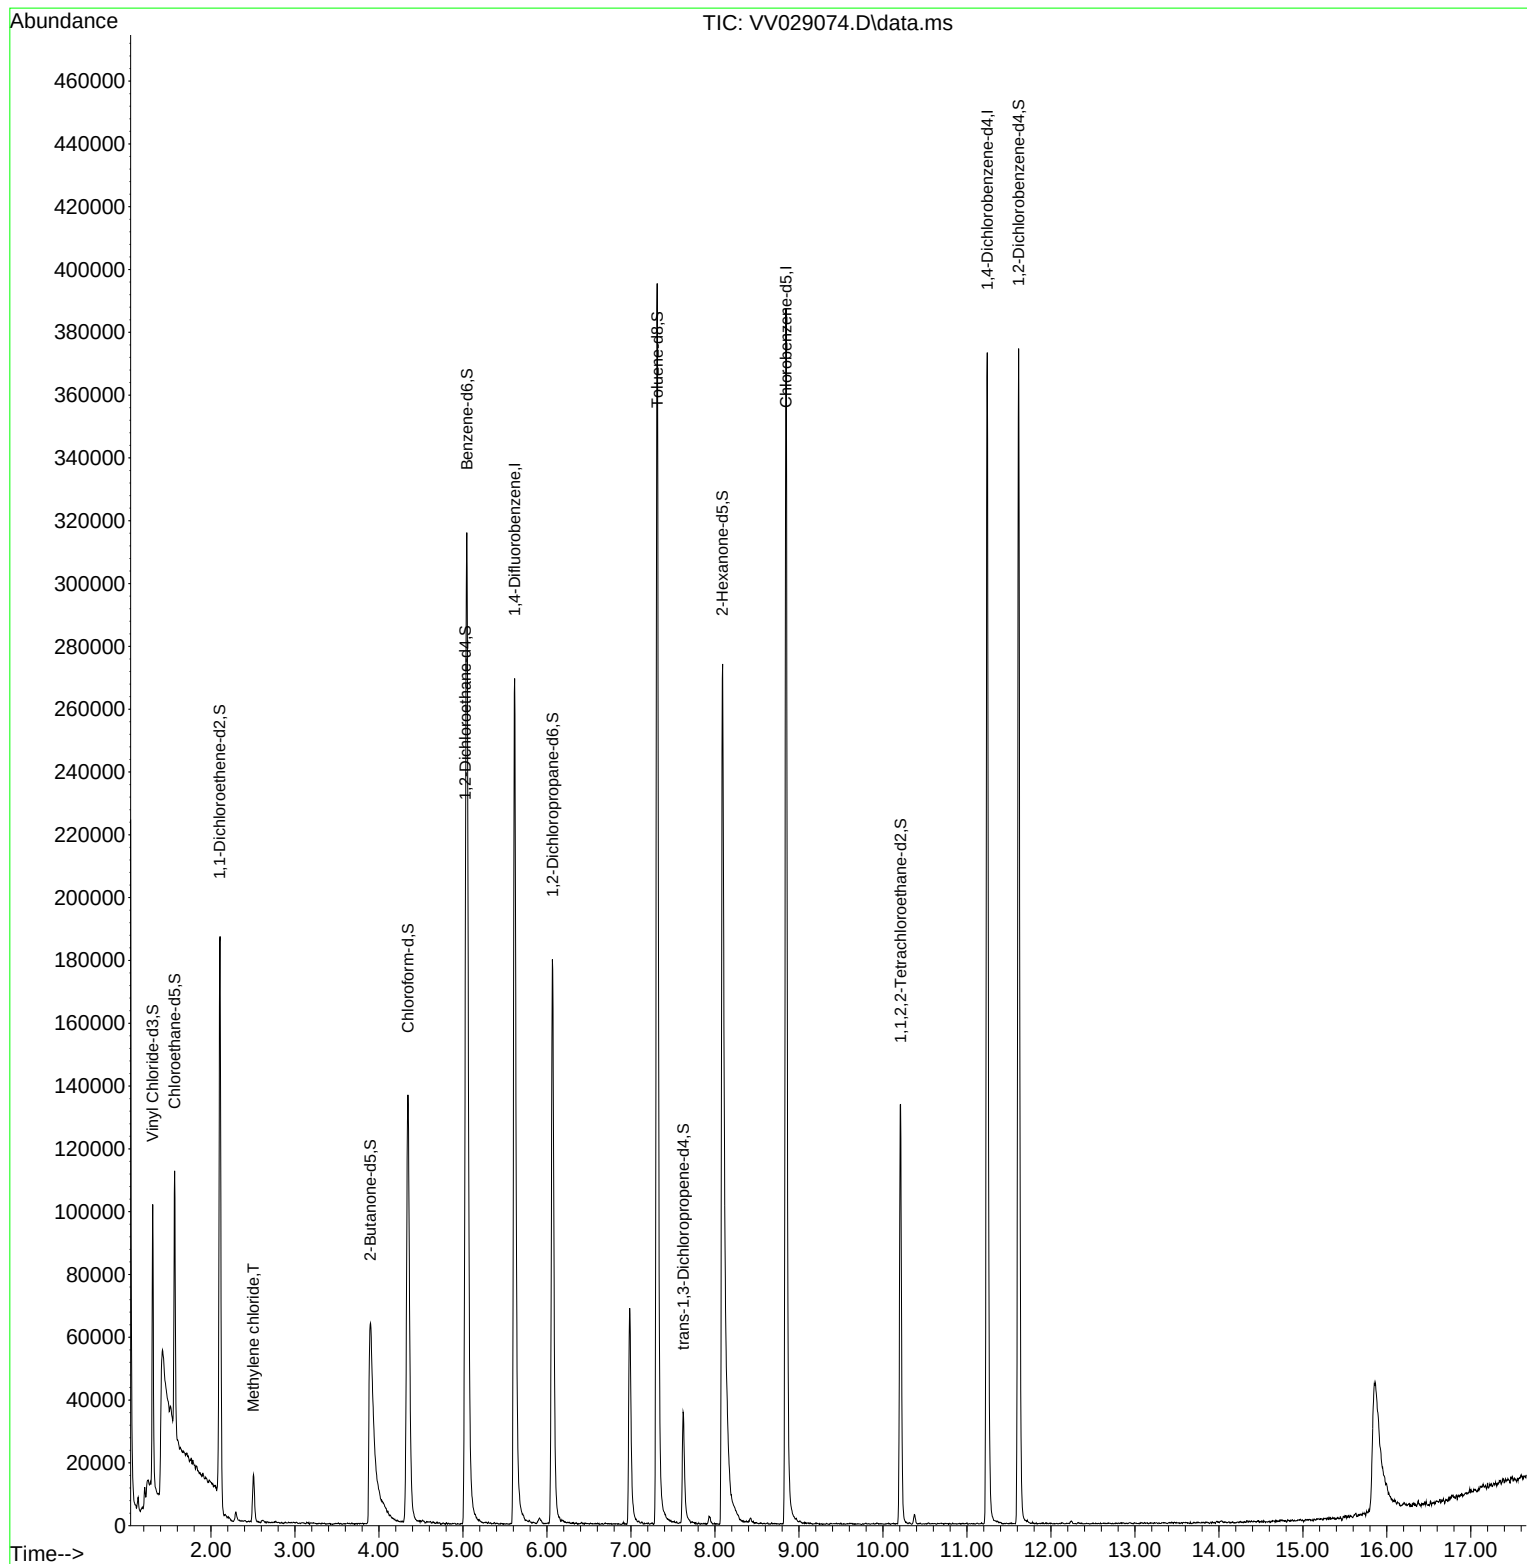

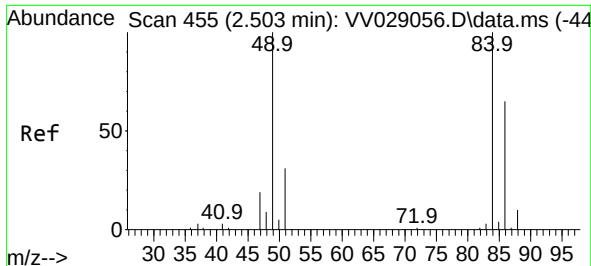

#16
Methylene chloride
Concen: 0.332 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV029074.D
Acq: 17 Nov 2022 19:25

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

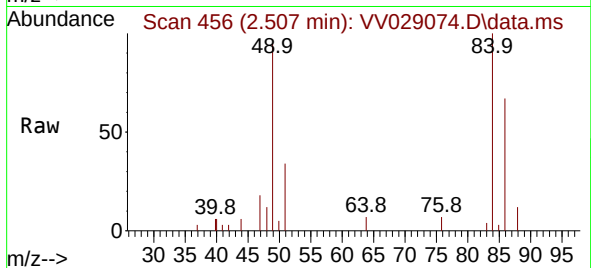

Tgt Ion: 84 Resp: 6827
Ion Ratio Lower Upper
84 100
86 67.3 45.8 85.0
49 95.2 75.5 140.1

