

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111722\
 Data File : VW029076.D
 Acq On : 17 Nov 2022 20:12
 Operator : SY/MD
 Sample : N5604-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Nov 18 01:45:25 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 01:37:41 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	266643	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	250952	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.243	152	116476	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	61098	3.759	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	75.200%
7) Chloroethane-d5	1.568	69	50620	3.542	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	70.800%
11) 1,1-Dichloroethene-d2	2.108	63	83089	2.805	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	56.000%#
20) 2-Butanone-d5	3.905	46	108244	39.779	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	79.560%
24) Chloroform-d	4.346	84	147838	4.430	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	88.600%
26) 1,2-Dichloroethane-d4	5.031	65	66334	4.418	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	88.400%
32) Benzene-d6	5.050	84	303912	4.057	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	81.200%
36) 1,2-Dichloropropane-d6	6.066	67	87947	4.205	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	84.000%
41) Toluene-d8	7.313	98	277403	4.114	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	82.200%
43) trans-1,3-Dichloroprop...	7.625	79	24243	3.554	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	71.000%
46) 2-Hexanone-d5	8.092	63	121198	41.621	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	83.240%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	66286	4.571	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	91.400%
66) 1,2-Dichlorobenzene-d4	11.616	152	105933	5.083	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.600%
Target Compounds						Qvalue
16) Methylene chloride	2.507	84	5421	0.260	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029076.D
Acq On : 17 Nov 2022 20:12
Operator : SY/MD
Sample : N5604-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001


Quant Time: Nov 18 01:45:25 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 01:37:41 2022
Response via : Initial Calibration

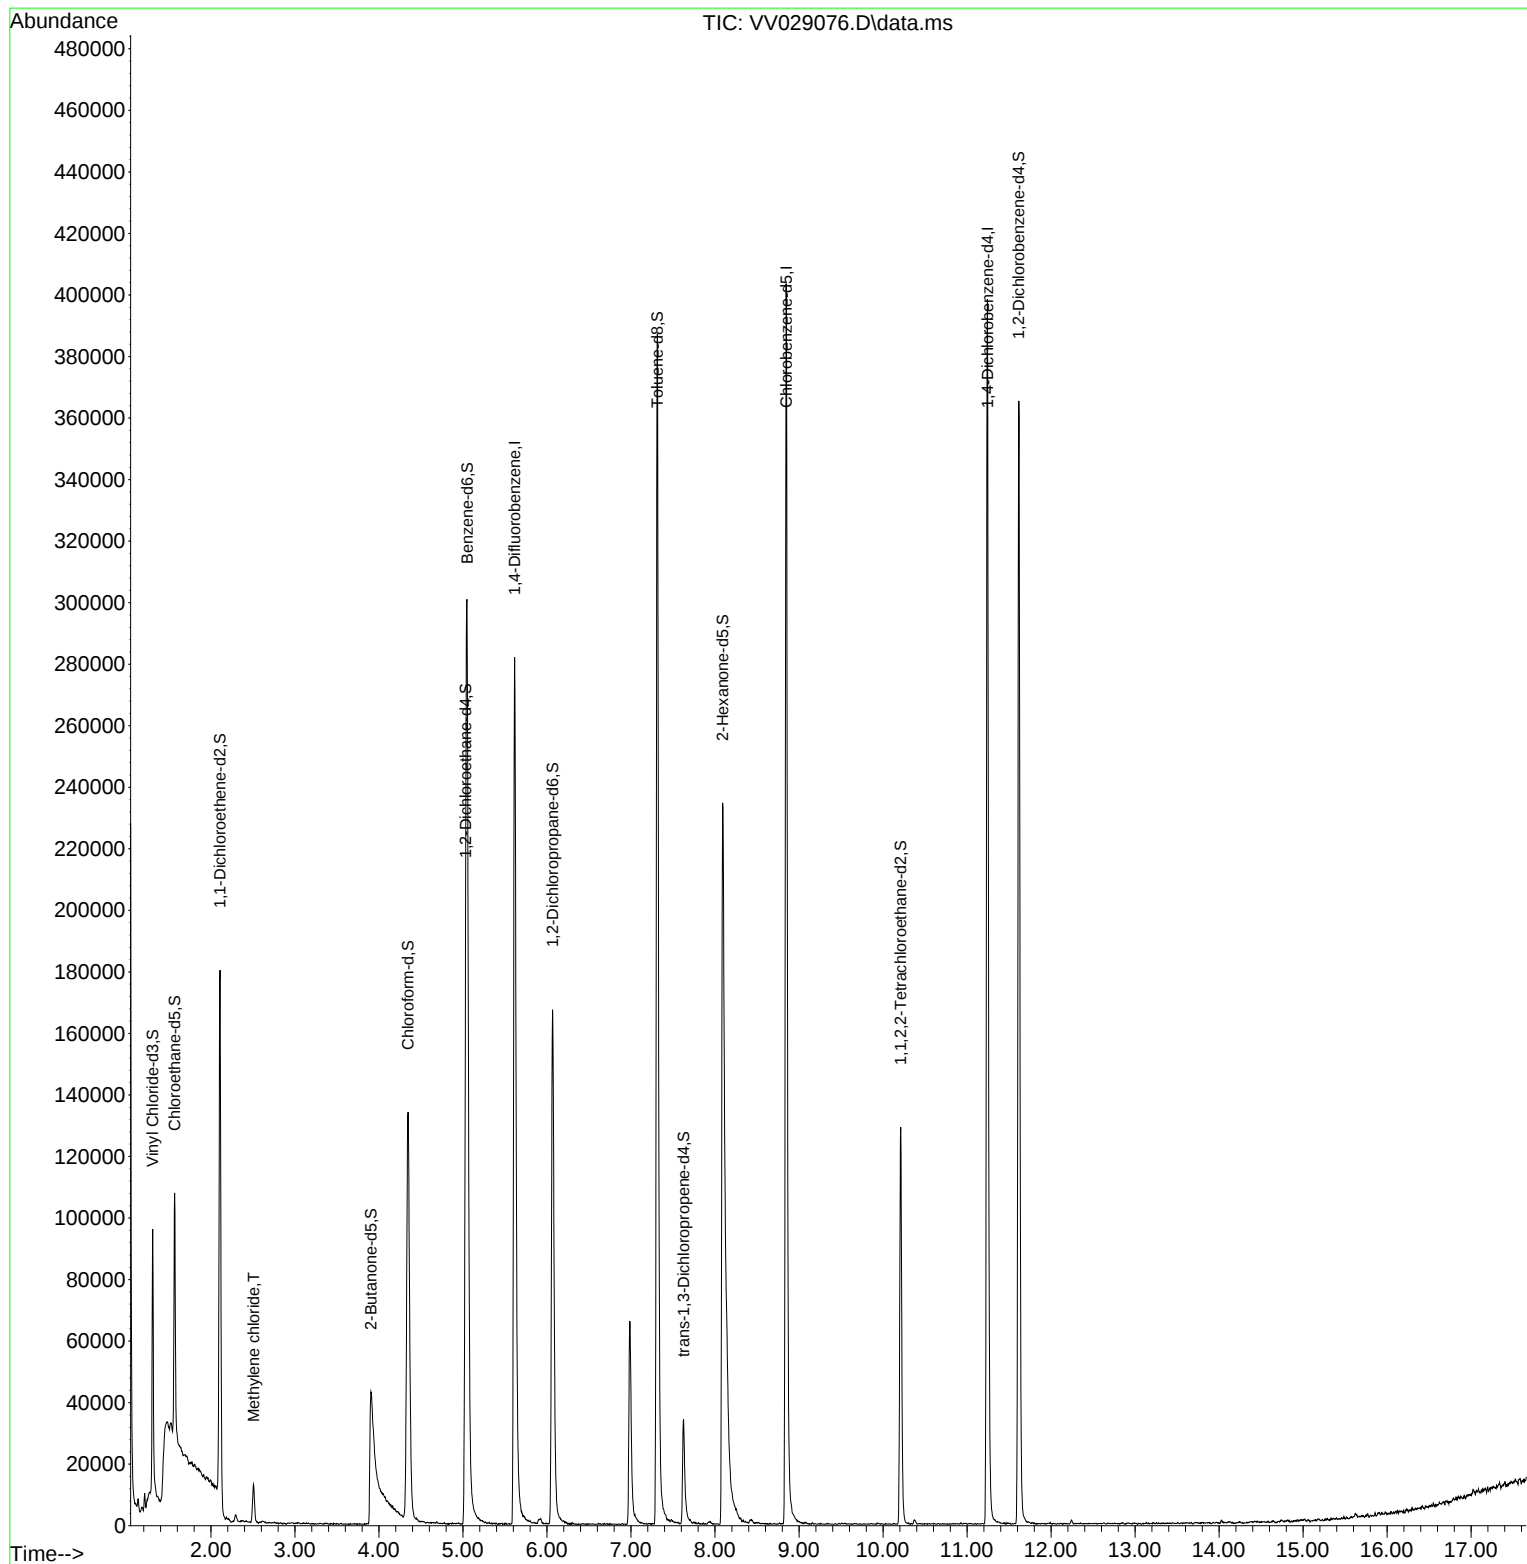

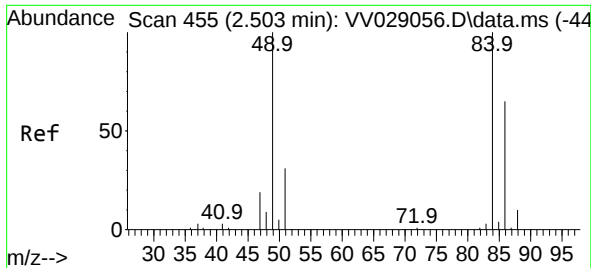

#16
Methylene chloride
Concen: 0.260 ug/L
RT: 2.507 min Scan# 4
Delta R.T. 0.003 min
Lab File: VV029076.D
Acq: 17 Nov 2022 20:12

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

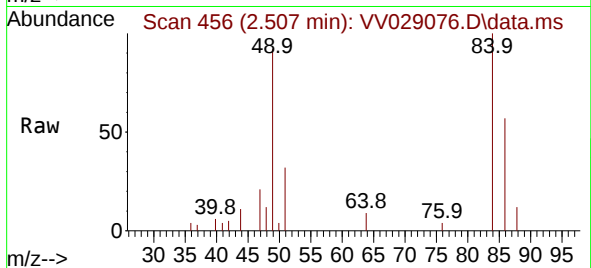

Tgt Ion: 84 Resp: 5421
Ion Ratio Lower Upper
84 100
86 57.3 45.8 85.0
49 91.9 75.5 140.1

