

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
 Data File : VV029059.D
 Acq On : 17 Nov 2022 13:28
 Operator : SY/MD
 Sample : N5592-05DL 200X
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H0AB0DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029059.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.307	76	83	103	rVB	93345	98556	6.34%	1.115%
2	1.520	126	149	155	rBV	15783	63665	4.09%	0.720%
3	1.561	156	162	174	rVB	83140	100602	6.47%	1.138%
4	2.105	320	331	357	rVB3	221154	372302	23.94%	4.211%
5	2.503	444	455	469	rBV	36872	61645	3.96%	0.697%
6	3.925	885	897	944	rBV2	53676	284170	18.27%	3.214%
7	4.343	1007	1027	1055	rBV3	137952	362184	23.29%	4.097%
8	5.043	1229	1245	1289	rBV2	338609	847930	54.52%	9.592%
9	5.613	1410	1422	1442	rBV	260738	539671	34.70%	6.105%
10	5.912	1501	1515	1545	rBV	180687	374426	24.07%	4.235%
11	6.066	1550	1563	1590	rVV	183509	381042	24.50%	4.310%
12	6.982	1837	1848	1878	rBV2	85041	173260	11.14%	1.960%
13	7.310	1939	1950	1988	rBV	420682	760616	48.90%	8.604%
14	7.622	2034	2047	2069	rBV2	45719	89883	5.78%	1.017%
15	7.969	2138	2155	2182	rBV	923245	1555392	100.00%	17.594%
16	8.092	2183	2193	2242	rVV	306051	685690	44.08%	7.756%
17	8.847	2412	2428	2455	rBV	375438	637889	41.01%	7.216%
18	10.210	2840	2852	2875	rBV	142486	231469	14.88%	2.618%
19	11.243	3162	3173	3196	rBV	363463	601911	38.70%	6.809%
20	11.616	3276	3289	3318	rBV	375643	618124	39.74%	6.992%




Sum of corrected areas: 8840427

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029059.D
Acq On : 17 Nov 2022 13:28
Operator : SY/MD
Sample : N5592-05DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

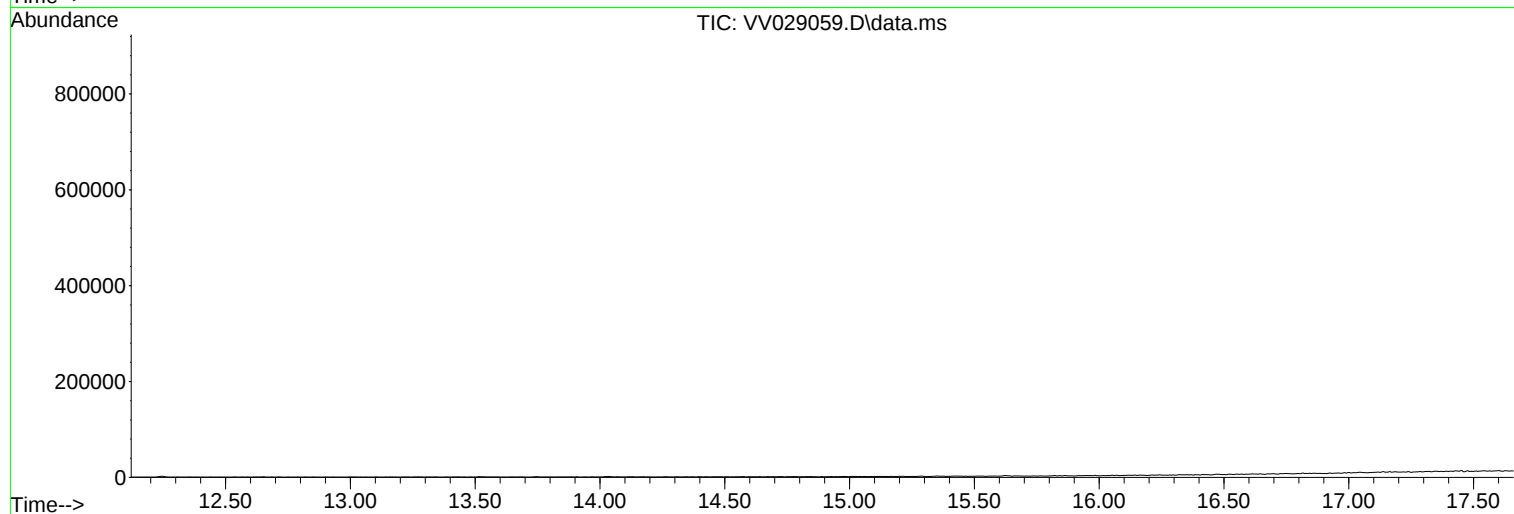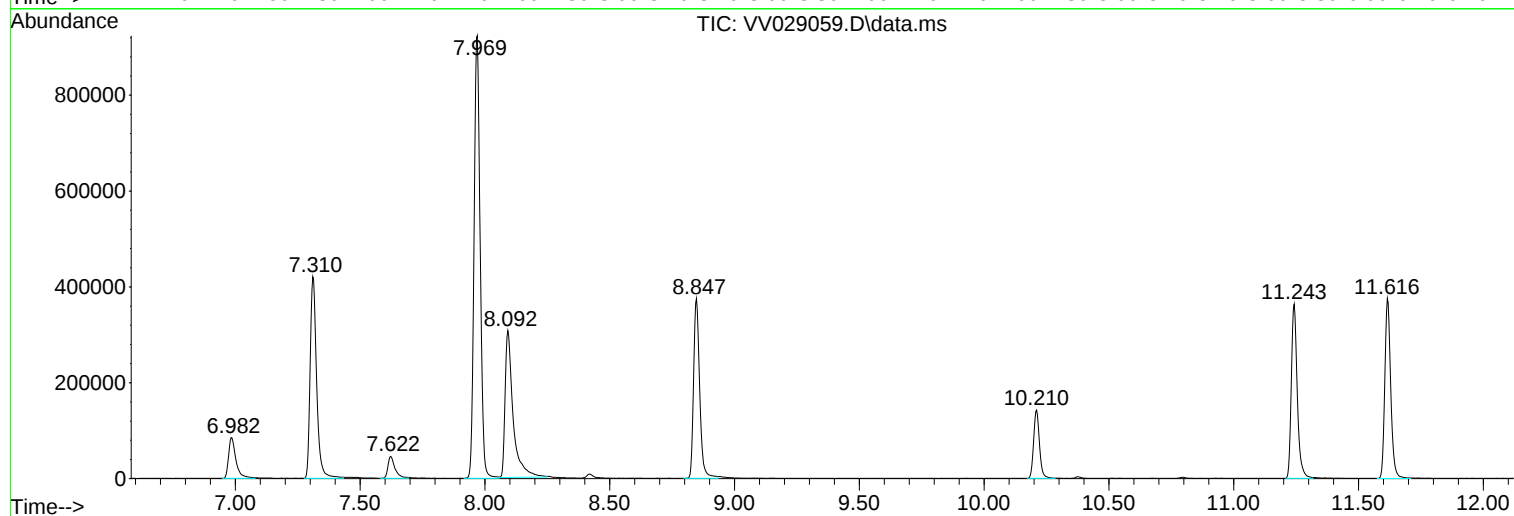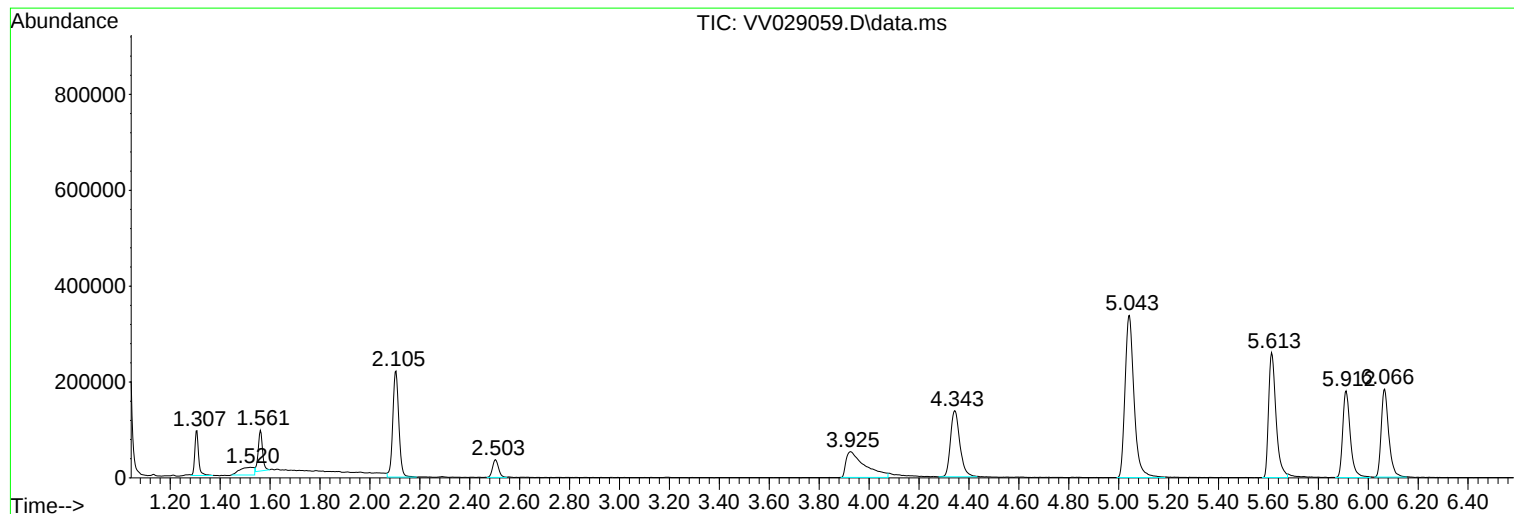

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029059.D
Acq On : 17 Nov 2022 13:28
Operator : SY/MD
Sample : N5592-05DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029059.D
Acq On : 17 Nov 2022 13:28
Operator : SY/MD
Sample : N5592-05DL 200X
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H0AB0DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc