

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
 Data File : VV029078.D
 Acq On : 17 Nov 2022 20:57
 Operator : SY/MD
 Sample : N5687-02
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCC5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV029078.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.243	58	63	73	rBV6	5507	10577	1.37%	0.162%
2	1.307	77	83	100	rVB	84751	92922	12.08%	1.425%
3	1.420	103	118	157	rBV2	56775	338588	44.01%	5.191%
4	1.568	158	164	176	rVB	81083	99032	12.87%	1.518%
5	2.108	322	332	360	rVB	175118	290910	37.81%	4.460%
6	3.902	881	890	922	rBV	33699	148215	19.27%	2.272%
7	4.342	1013	1027	1059	rVB2	129524	336701	43.77%	5.162%
8	5.043	1228	1245	1277	rBV2	298984	769335	100.00%	11.796%
9	5.616	1409	1423	1454	rBV	247974	523184	68.00%	8.022%
10	6.066	1548	1563	1593	rBV	166338	355021	46.15%	5.443%
11	6.985	1839	1849	1870	rBV	66585	131966	17.15%	2.023%
12	7.313	1938	1951	1973	rBV	371185	677961	88.12%	10.395%
13	7.625	2037	2048	2079	rBV	35735	72645	9.44%	1.114%
14	8.091	2181	2193	2260	rBV3	203572	697794	90.70%	10.699%
15	8.847	2415	2428	2460	rBV	357307	619761	80.56%	9.502%
16	10.210	2840	2852	2875	rBV	130127	218778	28.44%	3.354%
17	10.378	2894	2904	2915	rBV	7930	13340	1.73%	0.205%
18	11.242	3162	3173	3196	rBV	331991	549129	71.38%	8.419%
19	11.615	3277	3289	3312	rBV	348938	576359	74.92%	8.837%




Sum of corrected areas: 6522218

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029078.D
Acq On : 17 Nov 2022 20:57
Operator : SY/MD
Sample : N5687-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

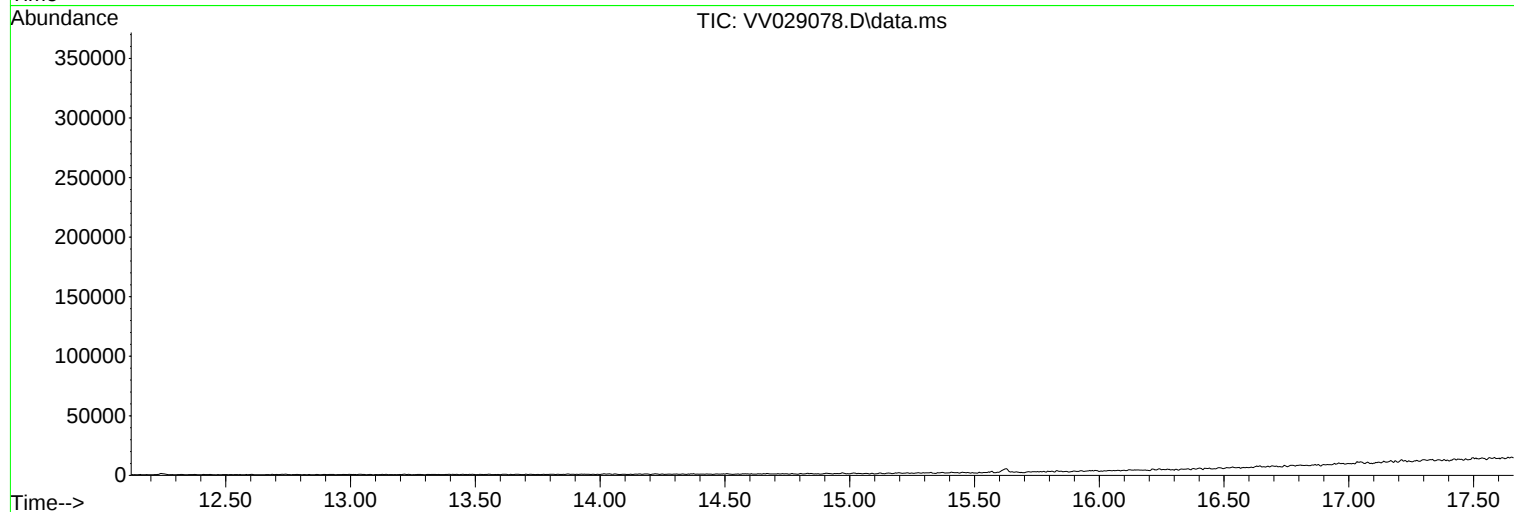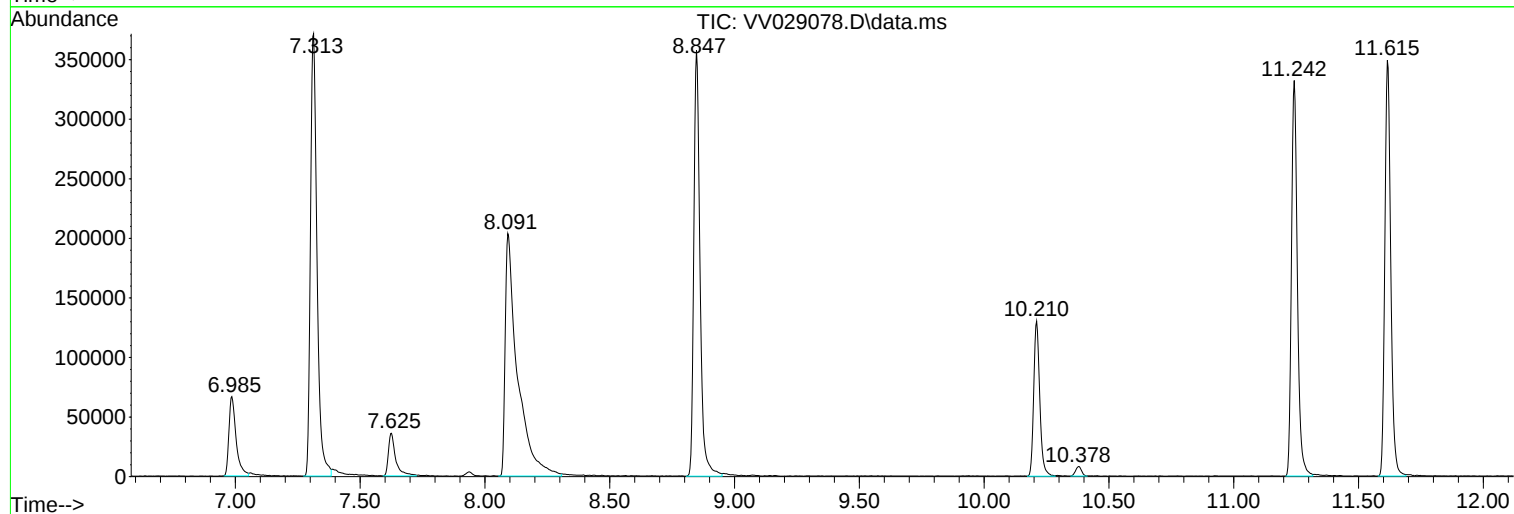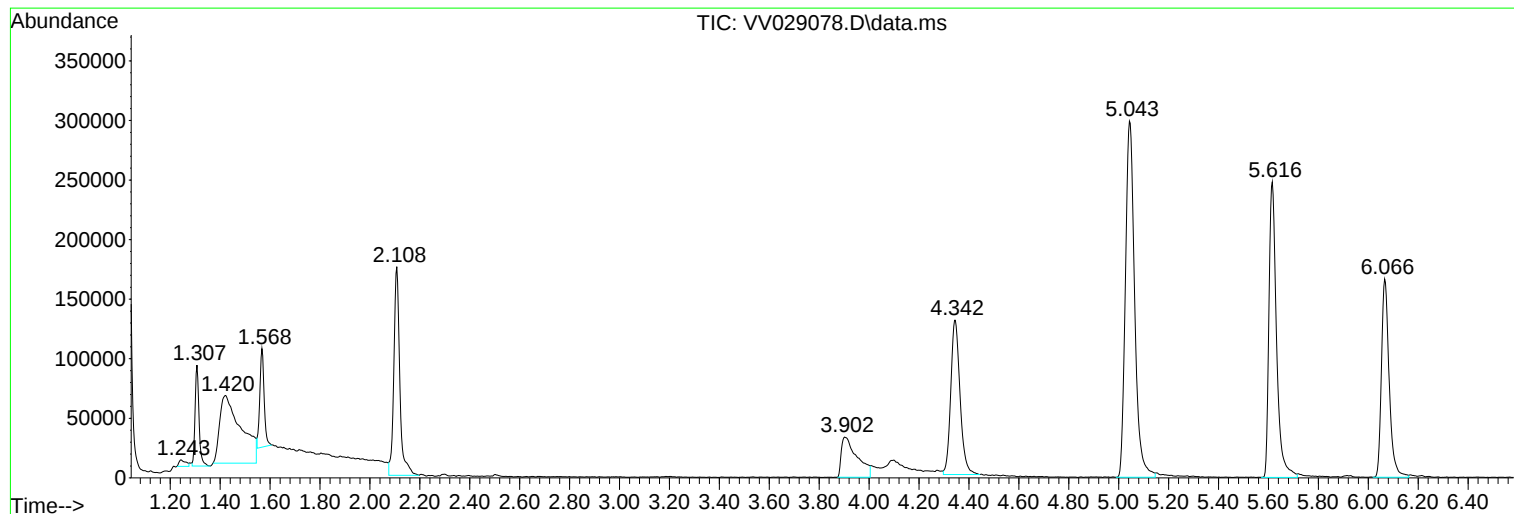

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029078.D
Acq On : 17 Nov 2022 20:57
Operator : SY/MD
Sample : N5687-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCC5










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.420	3.24 ug/L	338588	1,4-Difluorobenzene	5.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
3			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
4			Sulfur dioxide	64	O2S	007446-09-5	5
5			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4

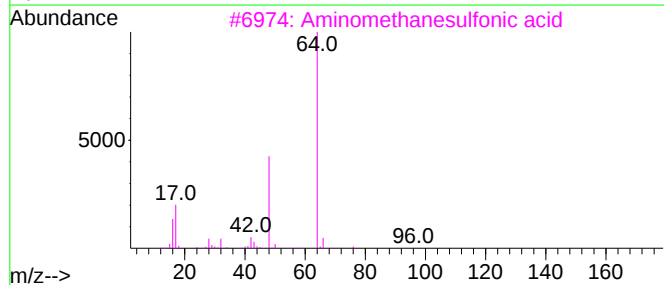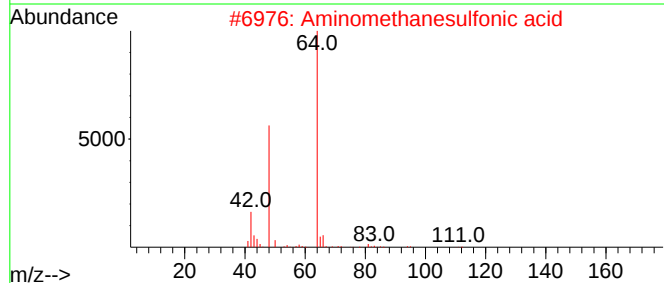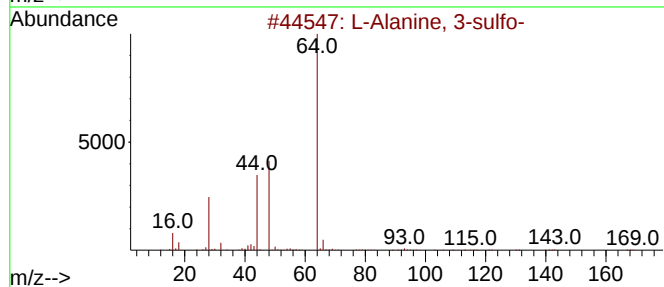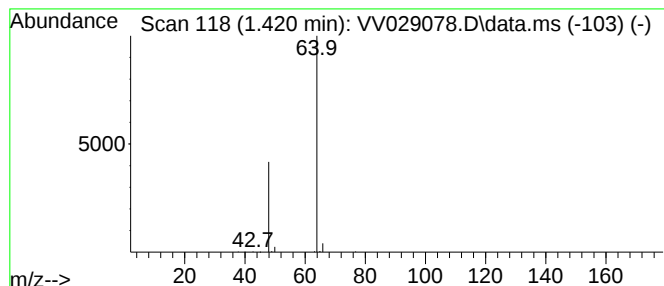

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029078.D
Acq On : 17 Nov 2022 20:57
Operator : SY/MD
Sample : N5687-02
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCC5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.420	3.2	ug/L	338588	1	5.616	523184	5.0