

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
 Data File : VV029089.D
 Acq On : 18 Nov 2022 01:47
 Operator : SY/MD
 Sample : N5648-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 H46D7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV029089.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.311	75	84	102	rVB2	266690	316335	6.14%	2.180%
2	1.397	102	111	139	rBV	49883	196488	3.81%	1.354%
3	1.568	158	164	177	rVB	82288	93487	1.81%	0.644%
4	2.108	322	332	347	rVB	175182	270451	5.25%	1.864%
5	2.761	521	535	555	rBV2	320189	631913	12.26%	4.356%
6	3.902	874	890	938	rBV	2079829	5152203	100.00%	35.512%
7	4.343	1010	1027	1061	rVB	129688	341936	6.64%	2.357%
8	5.044	1229	1245	1281	rBV2	310942	821868	15.95%	5.665%
9	5.613	1411	1422	1450	rBV	261168	545510	10.59%	3.760%
10	5.908	1498	1514	1550	rBV	1104528	2175218	42.22%	14.993%
11	6.066	1550	1563	1594	rVB	171389	362393	7.03%	2.498%
12	6.986	1839	1849	1878	rBV	76246	150277	2.92%	1.036%
13	7.310	1936	1950	1987	rBV	387050	698655	13.56%	4.816%
14	7.622	2037	2047	2064	rBV	40500	77885	1.51%	0.537%
15	8.088	2179	2192	2228	rBV2	277897	699839	13.58%	4.824%
16	8.847	2417	2428	2459	rBV	373485	634060	12.31%	4.370%
17	10.211	2840	2852	2874	rBV	135737	223454	4.34%	1.540%
18	11.243	3157	3173	3200	rBV	345039	561559	10.90%	3.871%
19	11.616	3278	3289	3310	rBV	344877	554638	10.77%	3.823%




Sum of corrected areas: 14508169

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029089.D
Acq On : 18 Nov 2022 01:47
Operator : SY/MD
Sample : N5648-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

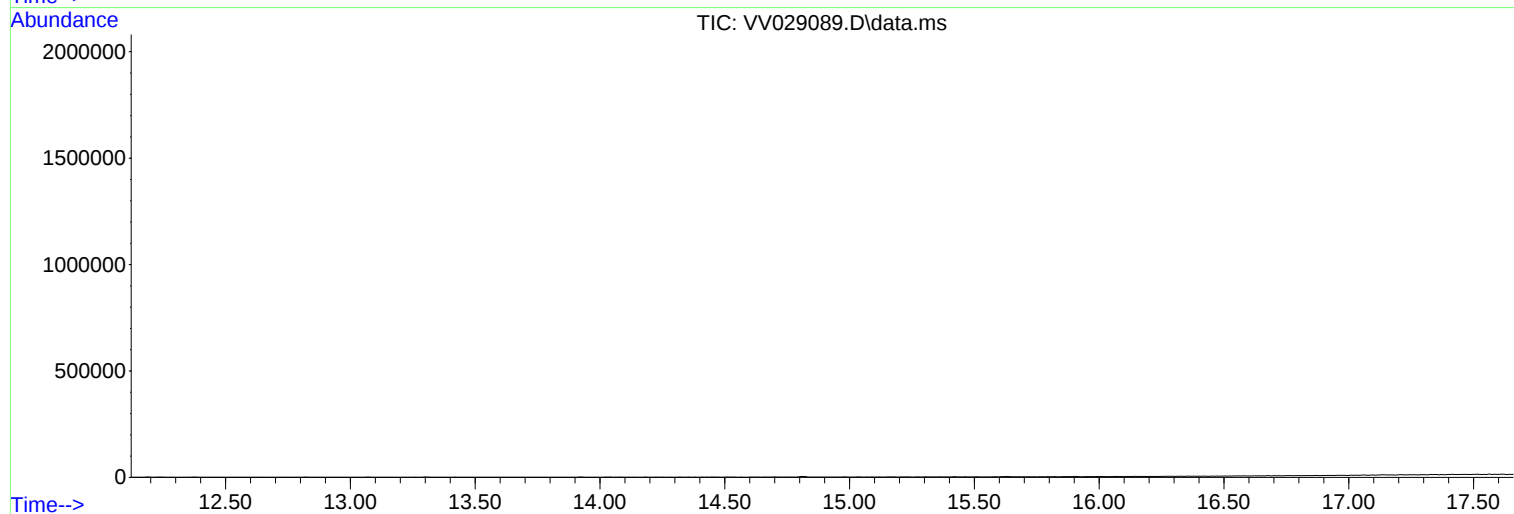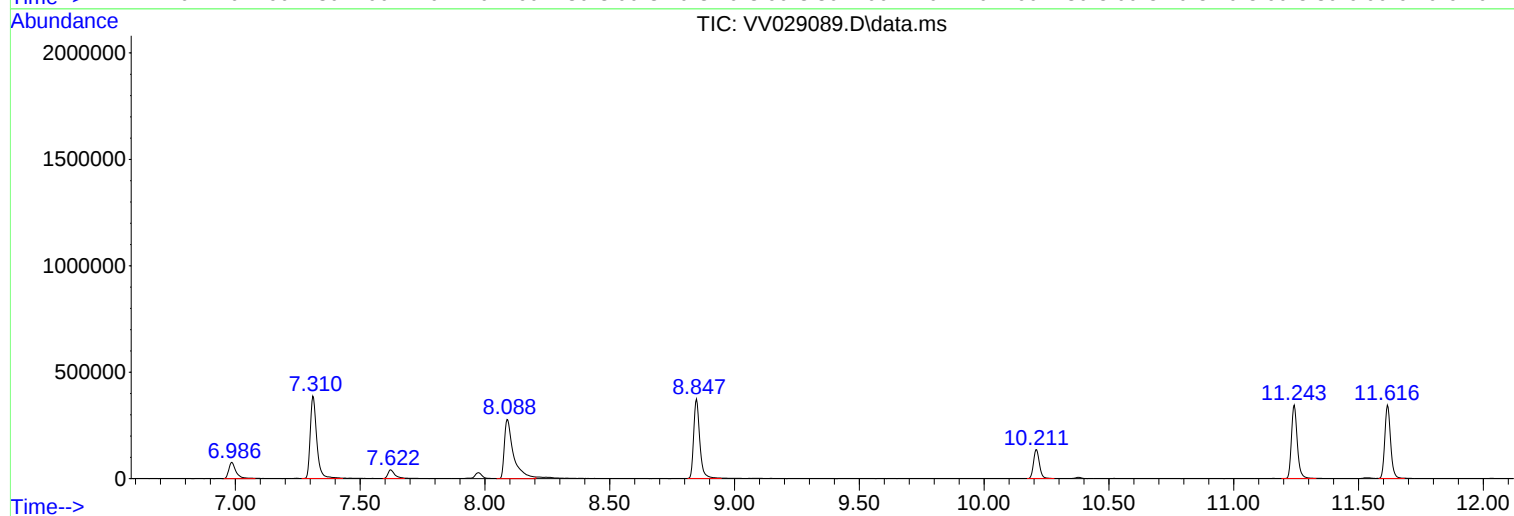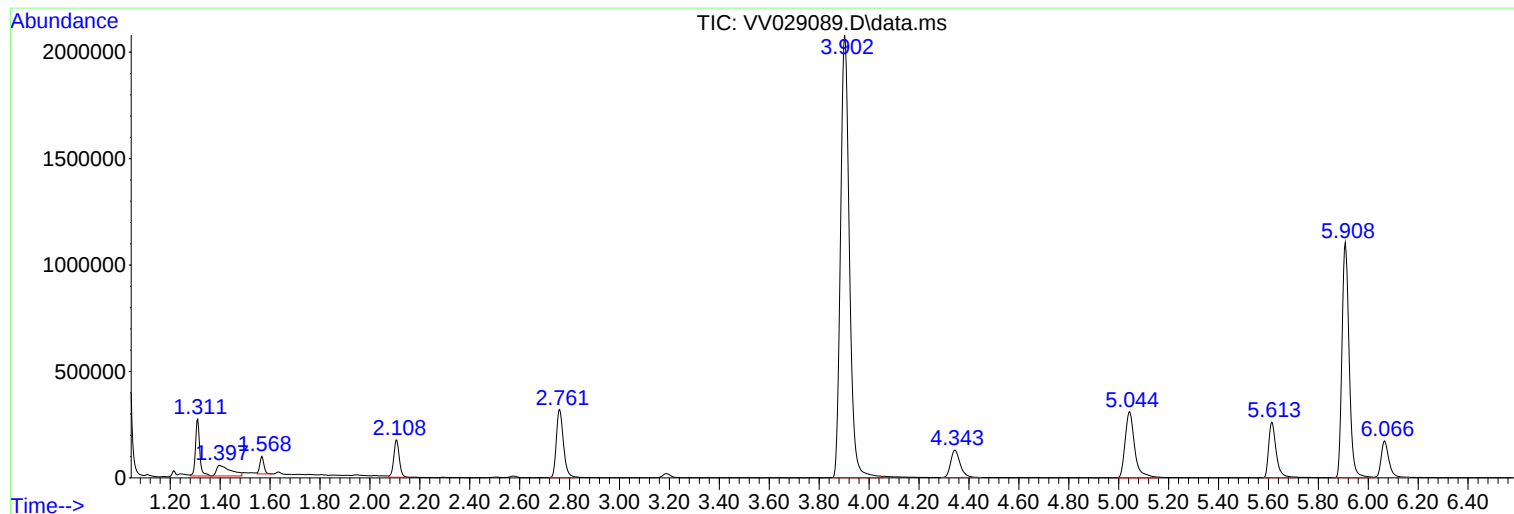

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029089.D
Acq On : 18 Nov 2022 01:47
Operator : SY/MD
Sample : N5648-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D7










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.397	1.80 ug/L	196488	1,4-Difluorobenzene	5.613

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			L-Alanine, 3-sulfo-	169	C3H7NO5S	000498-40-8	9
2			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	9
3			Sulfur dioxide	64	O2S	007446-09-5	4
4			Ethene, 1,1-difluoro-	64	C2H2F2	000075-38-7	4
5			Aminomethanesulfonic acid	111	CH5NO3S	013881-91-9	4

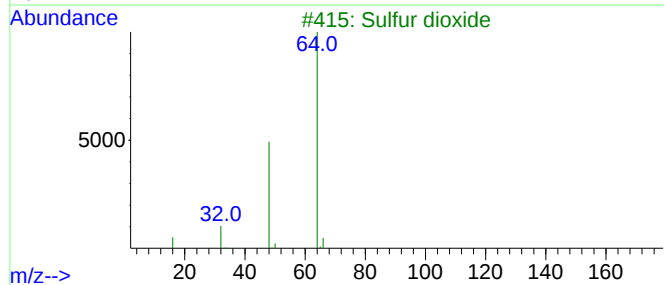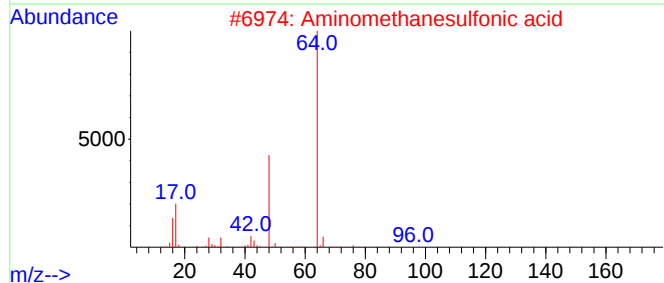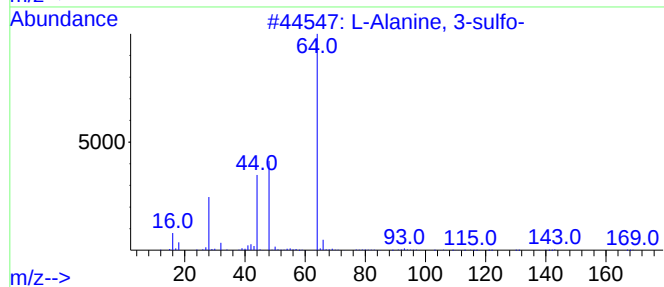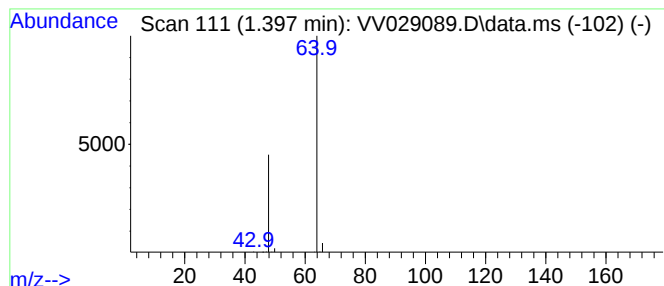

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029089.D
Acq On : 18 Nov 2022 01:47
Operator : SY/MD
Sample : N5648-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
H46D7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	1.397	1.8	ug/L	196488	1	5.613	545510	5.0