
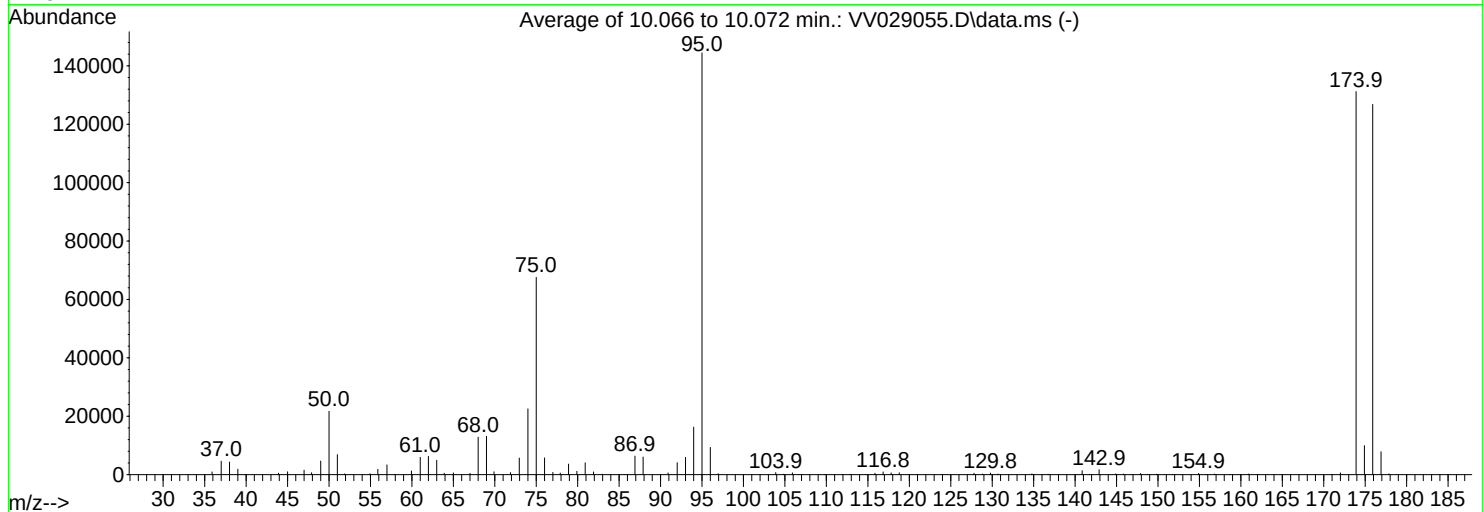


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111722\
Data File : VV029055.D
Acq On : 17 Nov 2022 09:51
Operator : SY/MD
Sample : BFB398
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB398

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Nov 18 04:35:43 2022

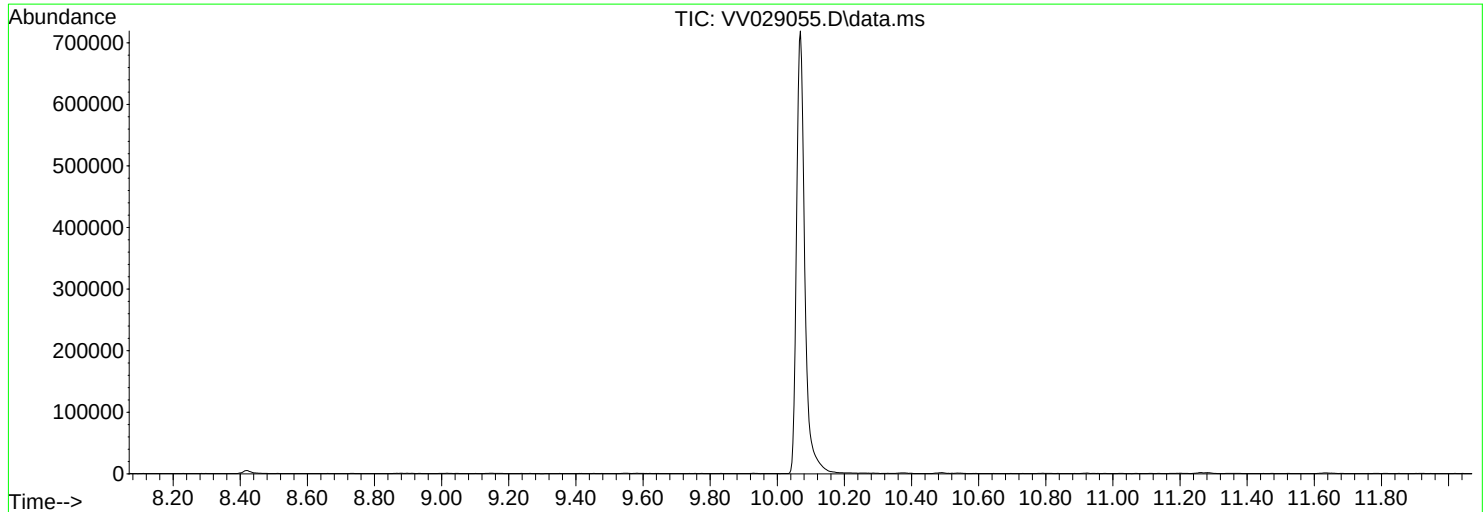

AutoFind: Scans 2807, 2808, 2809; Background Corrected with Scan 2795

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.0	21699	PASS
75	95	30	80	46.8	67573	PASS
95	95	100	100	100.0	144427	PASS
96	95	5	9	6.4	9294	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	90.8	131168	PASS
175	174	5	9	7.6	9927	PASS
176	174	95	105	96.6	126768	PASS
177	176	5	10	6.2	7823	PASS

m/z	Abundance
39.80	229.0
43.90	271.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
35.90	920.0
37.00	4893.0
38.00	4250.0
39.00	1985.0
39.90	293.0
43.90	748.0
45.00	973.0
46.00	103.0
47.00	1697.0
47.90	648.0
49.00	4700.0
50.00	22624.0
51.00	7047.0
51.90	296.0
55.00	376.0
55.90	1820.0
57.00	3582.0
57.90	115.0
59.90	1229.0
61.00	6139.0
62.00	6435.0
63.00	5102.0
63.90	531.0
65.00	665.0
67.00	446.0
68.00	13050.0
69.00	13314.0
69.90	982.0
71.90	657.0
73.00	5928.0
74.00	22368.0
75.00	69224.0
76.00	5881.0
77.00	813.0
78.00	602.0
78.90	3692.0
79.90	1161.0
80.90	4226.0
81.90	908.0
82.90	153.0
83.90	102.0
86.00	180.0
86.90	6470.0
87.90	5990.0
90.90	574.0
92.00	4395.0
93.00	5766.0
94.00	16289.0
95.00	146432.0
96.00	9417.0
96.90	361.0
103.90	671.0
104.80	197.0
105.90	595.0
109.80	104.0
111.90	115.0
112.80	128.0
114.90	132.0
115.80	533.0
116.80	986.0
117.80	604.0
118.80	578.0
127.80	497.0
128.90	209.0
129.80	485.0
130.70	174.0
134.80	289.0
136.70	204.0
140.80	1334.0
141.70	168.0
142.90	1673.0
144.90	313.0
145.80	200.0
147.90	352.0
148.70	115.0
149.80	183.0
151.80	108.0
154.90	433.0
156.70	246.0
160.90	250.0
171.90	629.0
173.90	129744.0
174.90	9928.0
175.90	125832.0
176.90	8150.0
177.80	282.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
35.90	951.0
37.00	4722.0
38.00	4501.0
39.00	1932.0
39.90	284.0
43.90	771.0
45.00	1035.0
46.00	118.0
47.00	1590.0
47.90	710.0
49.00	4812.0
50.00	22312.0
51.00	7062.0
51.90	290.0
54.90	351.0
55.90	1873.0
57.00	3445.0
60.00	1291.0
61.00	6104.0
62.00	6410.0
63.00	5068.0
63.90	538.0
65.00	675.0
67.00	446.0
68.00	13203.0
69.00	13643.0
69.90	969.0
71.90	707.0
72.90	5827.0
74.00	23232.0
75.00	69400.0
76.00	5843.0
77.00	783.0
77.90	565.0
78.90	3737.0
79.90	1207.0
80.90	4191.0
81.90	957.0
83.00	174.0
86.00	183.0
86.90	6531.0
87.90	6145.0
90.90	614.0
92.00	4302.0
93.00	6144.0
94.00	16856.0
95.00	148928.0
96.00	9572.0
97.00	333.0
103.90	761.0
104.80	197.0
105.90	628.0
110.90	110.0
111.90	110.0
112.90	147.0
114.70	116.0
115.90	551.0
116.90	956.0
117.80	626.0
118.80	692.0
127.80	543.0
128.80	211.0
129.80	594.0
130.70	244.0
134.80	304.0
136.80	189.0
140.80	1363.0
141.70	133.0
142.90	1768.0
144.90	306.0
145.80	210.0
146.80	132.0
147.90	381.0
148.70	118.0
149.80	179.0
154.90	460.0
155.80	106.0
156.80	254.0
161.00	230.0
170.90	129.0
172.00	639.0
173.90	135232.0
174.90	10301.0
175.90	130448.0
176.90	8079.0
177.90	274.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398

m/z	Abundance
35.90	943.0
37.00	4180.0
38.00	4218.0
39.00	1741.0
39.90	308.0
43.90	849.0
45.00	985.0
46.00	126.0
47.00	1341.0
47.90	635.0
49.00	4528.0
50.00	20160.0
51.00	6463.0
51.90	273.0
54.90	284.0
55.90	1710.0
57.00	3023.0
60.00	1201.0
61.00	5594.0
62.00	5864.0
63.00	4589.0
63.90	465.0
65.00	541.0
67.00	402.0
68.00	12206.0
69.00	12592.0
69.90	955.0
71.90	704.0
72.90	5290.0
74.00	21920.0
75.00	64096.0
76.00	5460.0
77.00	767.0
77.80	541.0
78.90	3425.0
79.90	1112.0
80.90	3762.0
81.90	874.0
83.00	136.0
85.70	176.0
86.90	6113.0
87.90	5912.0
90.90	577.0
92.00	3699.0
93.00	5810.0
94.00	15612.0
95.00	137920.0
96.00	8893.0
97.00	266.0
103.90	704.0
104.80	189.0
105.90	564.0
106.70	139.0
111.00	131.0
111.90	101.0
112.90	144.0
114.70	109.0
115.90	485.0
116.90	859.0
117.80	525.0
118.80	743.0
127.80	505.0
128.80	204.0
129.80	617.0
130.70	279.0
134.80	289.0
136.80	190.0
140.10	105.0
140.90	1356.0
142.90	1665.0
144.90	250.0
145.90	235.0
146.80	127.0
147.90	378.0
148.80	121.0
149.80	141.0
152.80	127.0
154.90	459.0
156.90	258.0
158.60	108.0
161.00	179.0
170.90	142.0
172.10	588.0
173.90	128528.0
174.90	9552.0
175.90	124024.0
176.90	7239.0
177.90	245.0

Instrument :
MSVOA_V
ClientSampleId :
BFB398