

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111725\
 Data File : VV039391.D
 Acq On : 17 Nov 2025 14:57
 Operator : SY/MD
 Sample : VV1117MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111725WMA.M

Title : VOC Analysis

Signal : TIC: VV039391.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.291	72	78	101	rVB	607161	800538	16.77%	2.304%
2	1.545	150	157	176	rVB	462105	677901	14.20%	1.951%
3	2.072	312	321	356	rVB	1028584	1875310	39.30%	5.397%
4	2.651	499	501	502	rBV2	4320	1845	0.04%	0.005%
5	2.854	560	564	568	rBV6	3603	3184	0.07%	0.009%
6	2.912	575	582	583	rBV7	4868	5122	0.11%	0.015%
7	2.953	589	595	601	rBV7	5454	8819	0.18%	0.025%
8	3.030	617	619	621	rBV3	2624	1529	0.03%	0.004%
9	3.207	671	674	676	rBV3	2958	1653	0.03%	0.005%
10	3.239	680	684	688	rVB6	4867	4084	0.09%	0.012%
11	3.262	689	691	693	rVV3	3633	1489	0.03%	0.004%
12	3.275	693	695	697	rVV3	2367	1271	0.03%	0.004%
13	3.326	705	711	714	rBV7	5866	6248	0.13%	0.018%
14	3.413	733	738	739	rBV5	4993	3220	0.07%	0.009%
15	3.474	755	757	763	rBV7	4581	4011	0.08%	0.012%
16	3.558	780	783	788	rBV7	3372	3102	0.06%	0.009%
17	3.603	795	797	798	rBV2	3696	1714	0.04%	0.005%
18	3.629	802	805	808	rVB5	3138	1840	0.04%	0.005%
19	3.648	808	811	812	rBV3	3226	1569	0.03%	0.005%
20	3.786	847	854	891	rBV	256956	813084	17.04%	2.340%
21	4.252	986	999	1033	rBV	656283	1892841	39.66%	5.447%
22	4.664	1125	1127	1130	rBV4	3697	1678	0.04%	0.005%
23	4.706	1138	1140	1142	rBV3	1877	912	0.02%	0.003%
24	4.722	1142	1145	1148	rBV4	4307	3323	0.07%	0.010%
25	4.956	1202	1218	1263	rBV2	1654765	4772371	100.00%	13.734%
26	5.532	1387	1397	1428	rBV	1140778	2561532	53.67%	7.372%
27	5.982	1526	1537	1565	rBV	968556	2139041	44.82%	6.156%
28	6.812	1793	1795	1798	rBV4	2932	2014	0.04%	0.006%
29	6.908	1815	1825	1852	rBV	490478	1000842	20.97%	2.880%
30	7.236	1916	1927	1969	rBV	1986292	3681313	77.14%	10.594%
31	7.545	2015	2023	2052	rBV	359665	705399	14.78%	2.030%
32	8.014	2160	2169	2203	rBV	988127	1920379	40.24%	5.526%
33	8.773	2395	2405	2439	rBV	1973348	3351948	70.24%	9.646%
34	9.297	2566	2568	2571	rVB4	2397	1214	0.03%	0.003%
35	9.320	2572	2575	2577	rBV3	2920	1705	0.04%	0.005%
36	9.361	2583	2588	2590	rBV6	5120	3991	0.08%	0.011%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111725\
 Data File : VV039391.D
 Acq On : 17 Nov 2025 14:57
 Operator : SY/MD
 Sample : VV1117MBL01
 Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK272

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111725WMA.M
 Title : VOC Analysis

37	9.570	2651	2653	2656	rBV3	2779	1870	0.04%	0.005%
38	9.728	2700	2702	2704	rBV3	3484	1593	0.03%	0.005%
39	9.812	2726	2728	2732	rBV5	2914	2402	0.05%	0.007%
40	10.001	2783	2787	2789	rBV5	3849	3192	0.07%	0.009%
41	10.014	2789	2791	2794	rVV4	2742	1918	0.04%	0.006%
42	10.140	2819	2830	2854	rBV	1431239	2302691	48.25%	6.627%
43	10.651	2988	2989	2992	rBV3	2501	926	0.02%	0.003%
44	10.940	3074	3079	3083	rBV7	4358	4055	0.08%	0.012%
45	11.024	3100	3105	3108	rBV6	4215	4198	0.09%	0.012%
46	11.172	3141	3151	3178	rBV	1883268	2997108	62.80%	8.625%
47	11.548	3257	3268	3293	rBV	1939977	3159201	66.20%	9.092%
48	12.519	3567	3570	3573	rBV4	5063	3252	0.07%	0.009%
49	12.828	3662	3666	3668	rBV5	4743	3427	0.07%	0.010%
50	13.191	3776	3779	3780	rBV3	3687	2136	0.04%	0.006%
51	14.188	4087	4089	4093	rBV5	3333	2915	0.06%	0.008%




Sum of corrected areas: 34748920

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111725\
Data File : VV039391.D
Acq On : 17 Nov 2025 14:57
Operator : SY/MD
Sample : VV1117MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

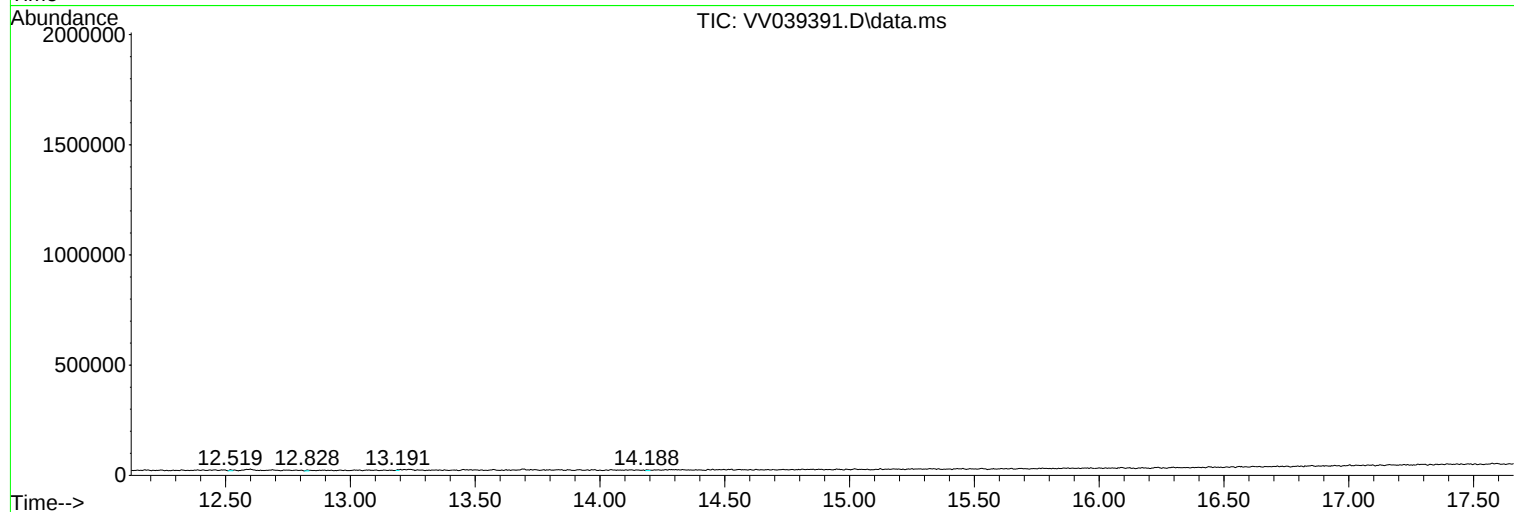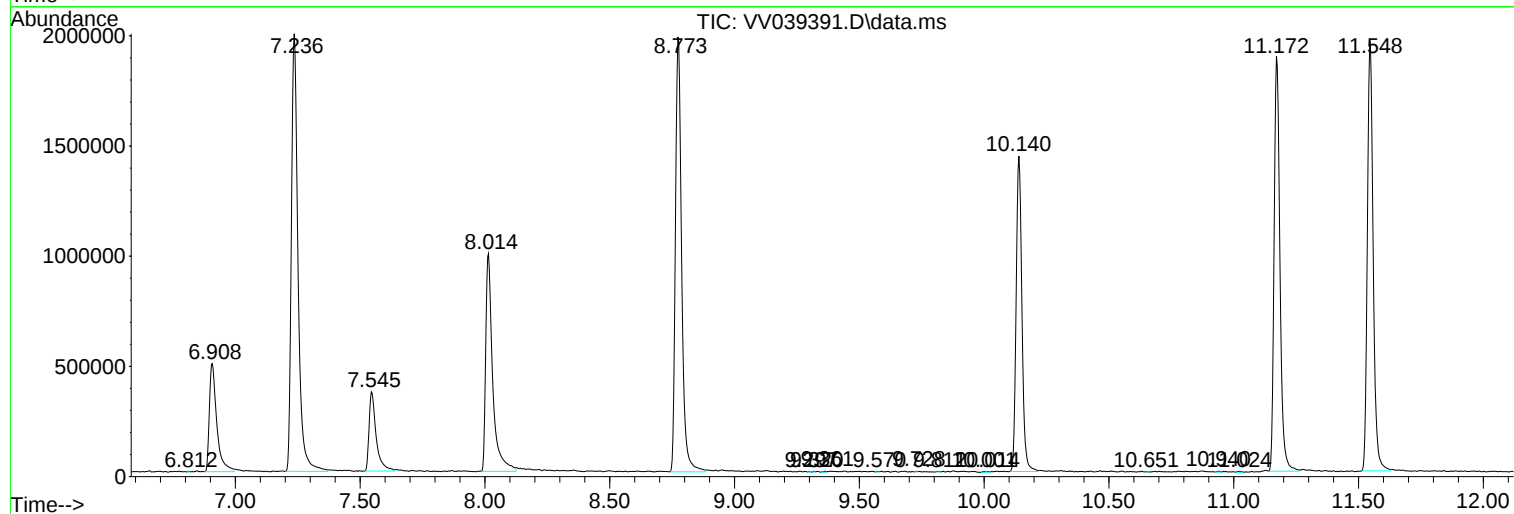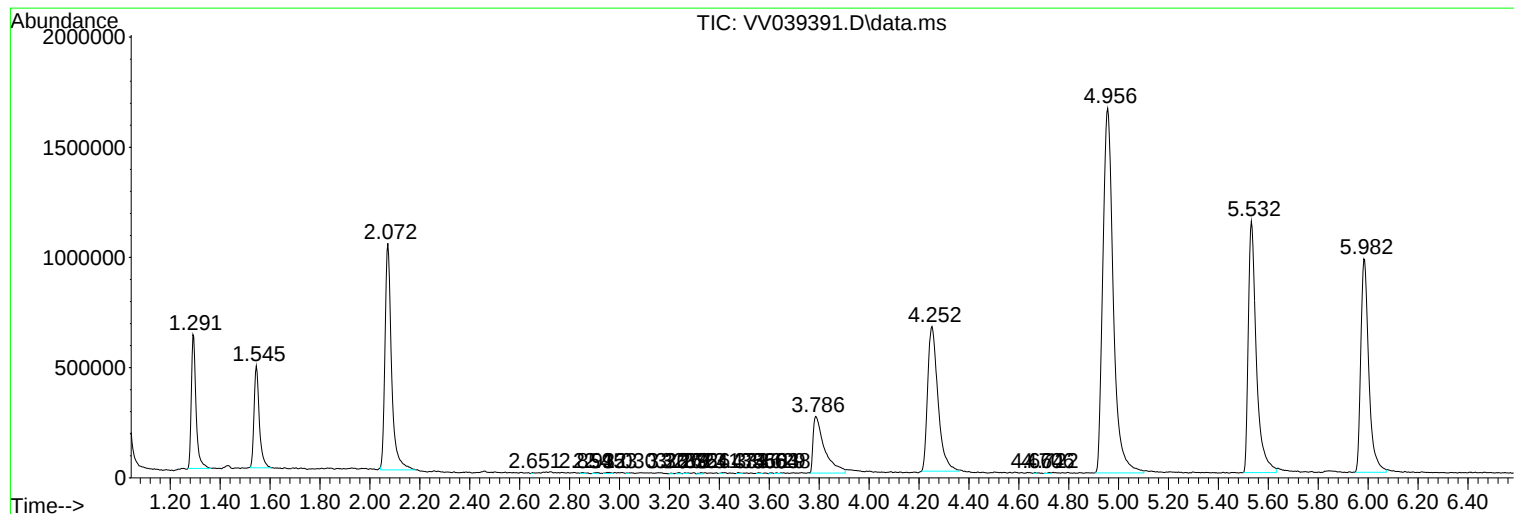

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111725\
Data File : VV039391.D
Acq On : 17 Nov 2025 14:57
Operator : SY/MD
Sample : VV1117MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111725\
Data File : VV039391.D
Acq On : 17 Nov 2025 14:57
Operator : SY/MD
Sample : VV1117MBL01
Misc : 5.00g/5.0mL/100uL/5.0mL/MSVOA_V/MEOH
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK272

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM111725WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc