
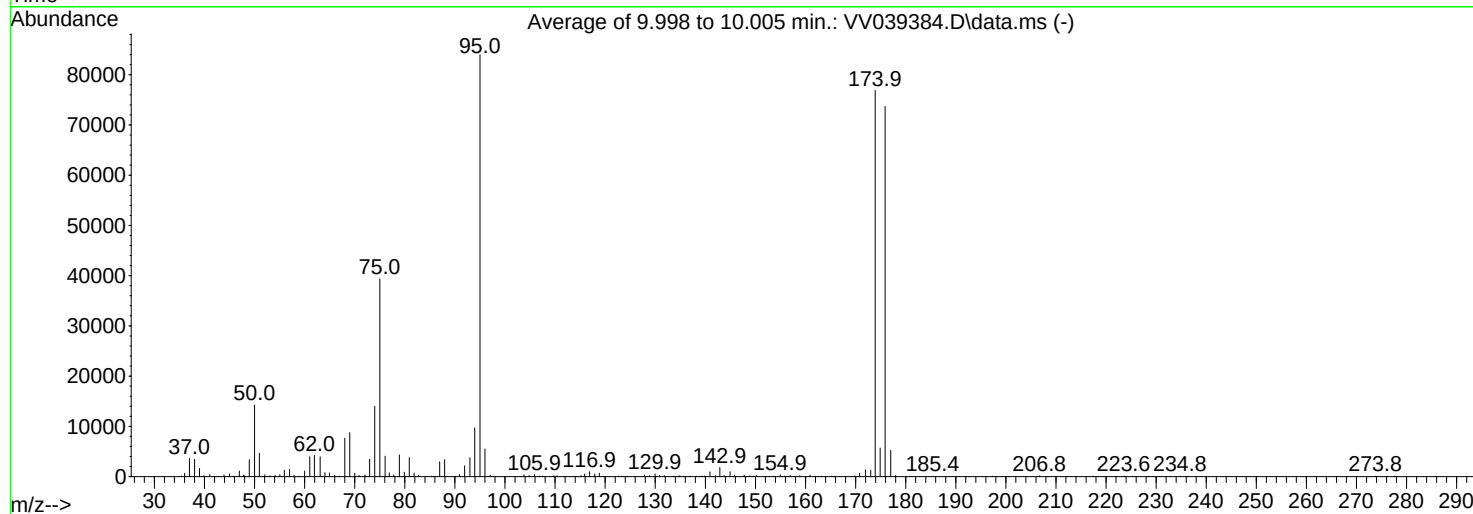


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\DATA\VV111725\
Data File : VV039384.D
Acq On : 17 Nov 2025 11:10
Operator : SY/MD
Sample : BFB207
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB207

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W111025S.M
Title : SW846 8260
Last Update : Tue Nov 11 03:48:21 2025

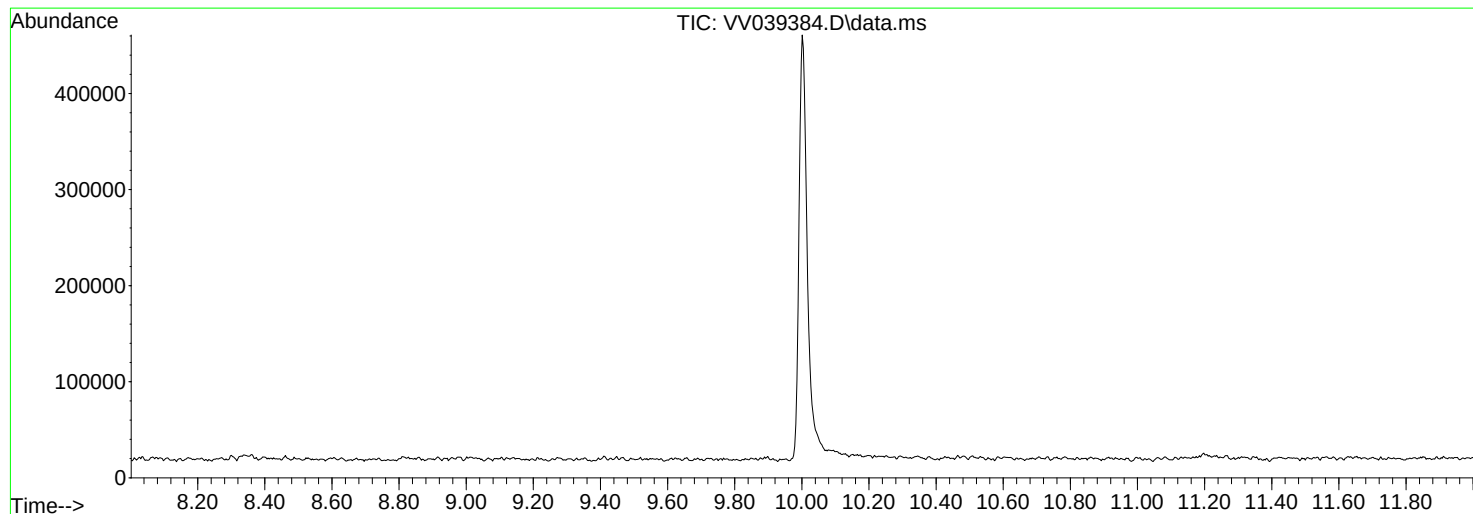

AutoFind: Scans 2786, 2787, 2788; Background Corrected with Scan 2771

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	14219	PASS
75	95	30	60	46.9	39363	PASS
95	95	100	100	100.0	83979	PASS
96	95	5	9	6.6	5510	PASS
173	174	0.00	2	1.6	1268	PASS
174	95	50	100	91.6	76896	PASS
175	174	5	9	7.4	5673	PASS
176	174	95	101	95.9	73707	PASS
177	176	5	9	7.1	5201	PASS