

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
 Data File : VV008629.D
 Acq On : 17 Nov 2018 15:13
 Operator : SY/MD
 Sample : J5990-05
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETO79

Quant Time: Nov 19 06:17:47 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 19 02:55:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	155342	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	140798	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	61284	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	29583	4.29	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	85.80%
7) Chloroethane-d5	1.58	69	26403	4.65	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	93.00%
11) 1,1-Dichloroethene-d2	2.13	63	44963	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.97	46	119339	48.33	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	96.66%
24) Chloroform-d	4.41	84	85782	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.09	65	46420	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.10	84	169946	4.63	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	92.60%
36) 1,2-Dichloropropane-d6	6.12	67	56785	4.79	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	95.80%
41) Toluene-d8	7.36	98	157022	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	91.00%
43) trans-1,3-Dichloropropene-	7.67	79	19167	4.24	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.80%
46) 2-Hexanone-d5	8.14	63	93939	45.91	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	91.82%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	37404	4.52	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	90.40%
64) 1,2-Dichlorobenzene-d4	11.68	152	55463	5.01	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	100.20%

Target Compounds


						Qvalue
8) Chloroethane	1.60	64	17638	3.06	ug/L	99
30) Cyclohexane	4.73	56	5010	0.25	ug/L	98
33) Benzene	5.15	78	129635	2.90	ug/L	100
35) Methylcyclohexane	6.18	83	2371	0.12	ug/L #	82
51) Chlorobenzene	8.93	112	105782	3.69	ug/L	99
56) Isopropylbenzene	9.98	105	31139	0.63	ug/L	100
63) 1,4-Dichlorobenzene	11.32	146	34100	1.73	ug/L	97
65) 1,2-Dichlorobenzene	11.69	146	4445	0.23	ug/L #	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
Data File : VV008629.D
Acq On : 17 Nov 2018 15:13
Operator : SY/MD
Sample : J5990-05
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETO79

Quant Time: Nov 19 06:17:47 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 19 02:55:31 2018
Response via : Initial Calibration

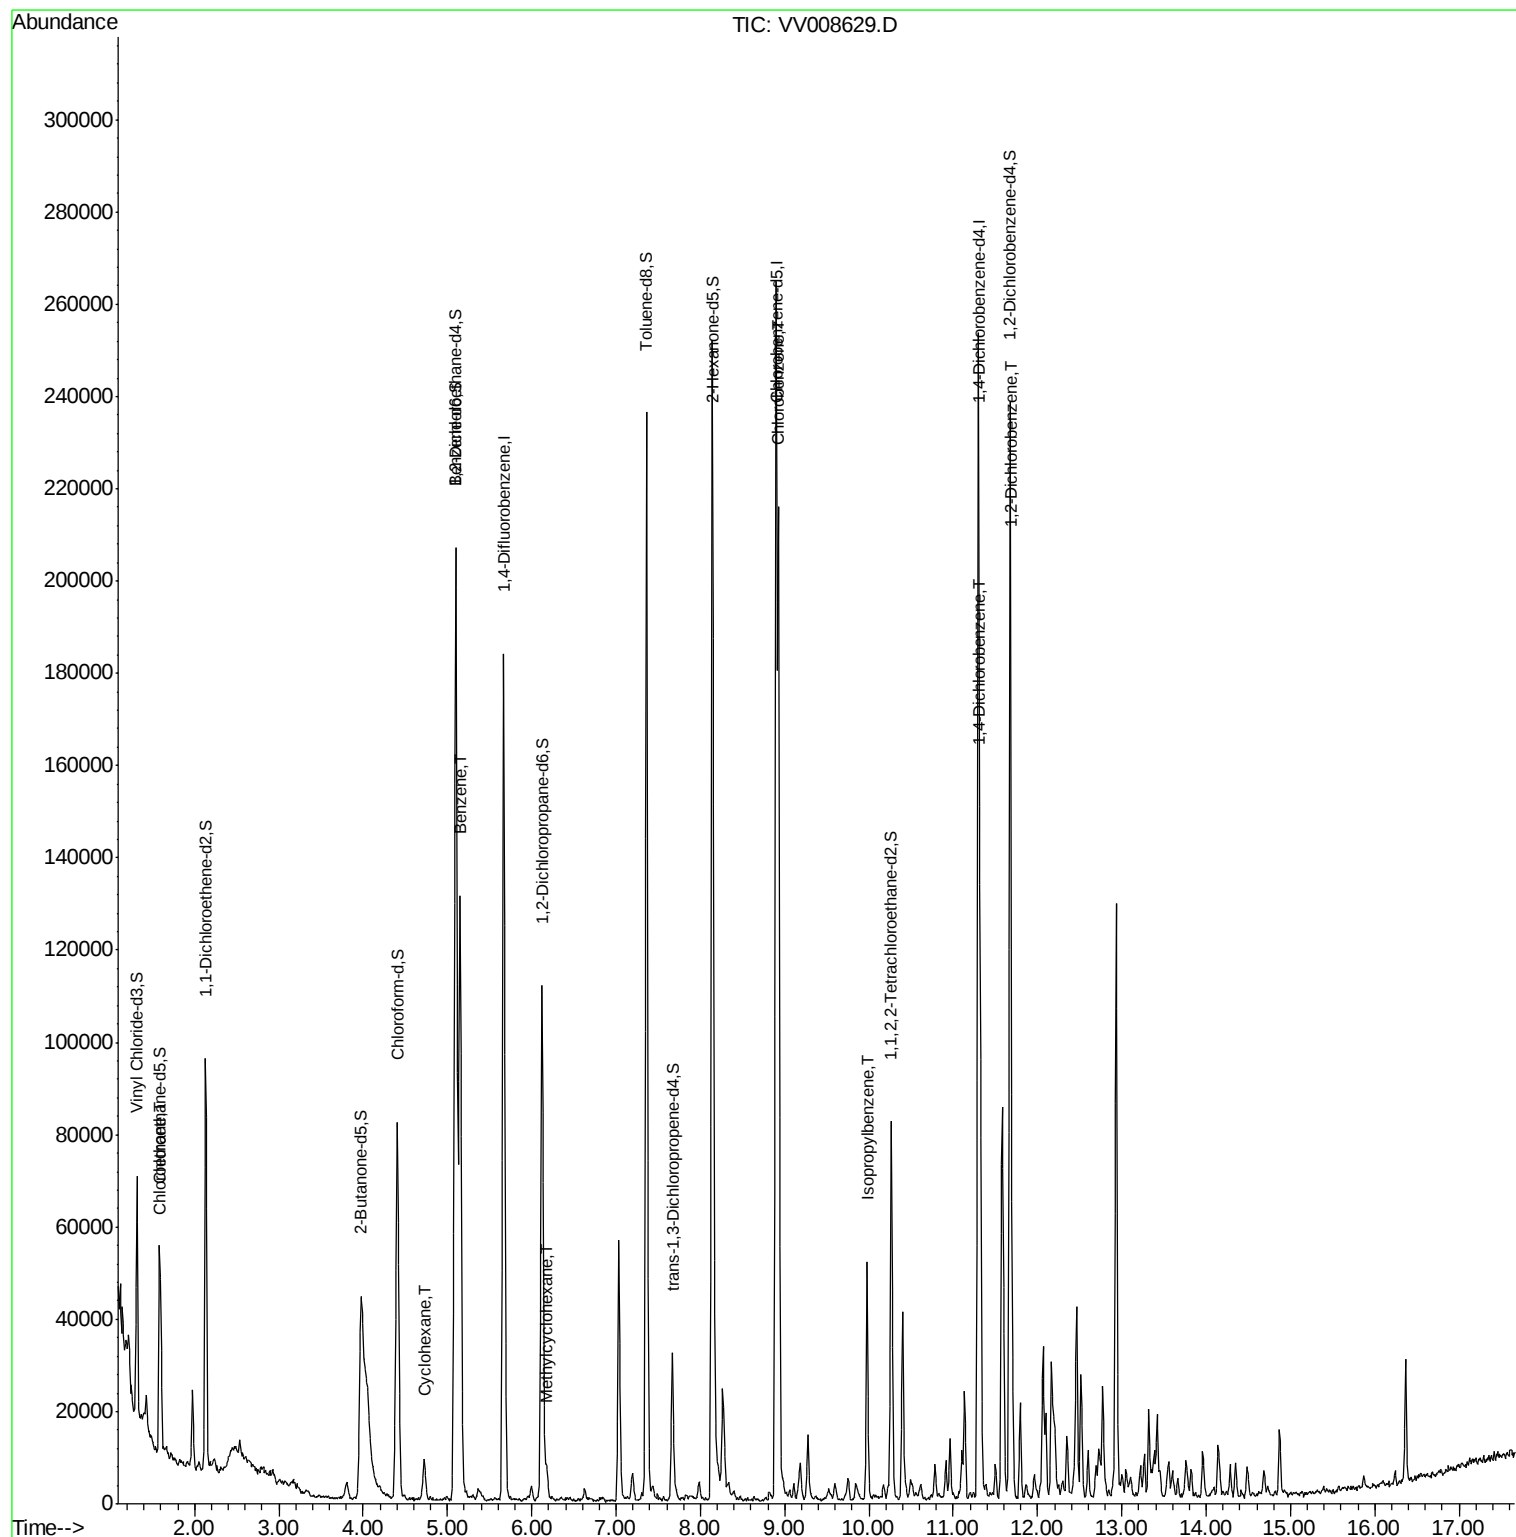

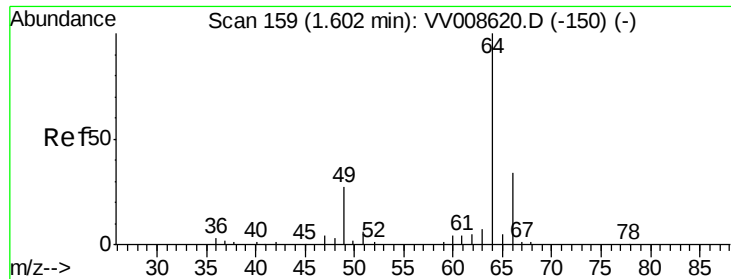

#8

Chloroethane

Concen: 3.06 ug/L

RT: 1.60 min Scan# 159

Delta R.T. 0.00 min

Lab File: VV008629.D

Acq: 17 Nov 2018 15:13

Instrument :

MSVOA_V

ClientSampled :





ETO79

Tgt Ion: 64 Resp: 17638

Ion Ratio Lower Upper

64 100

66 31.7 22.7 42.3

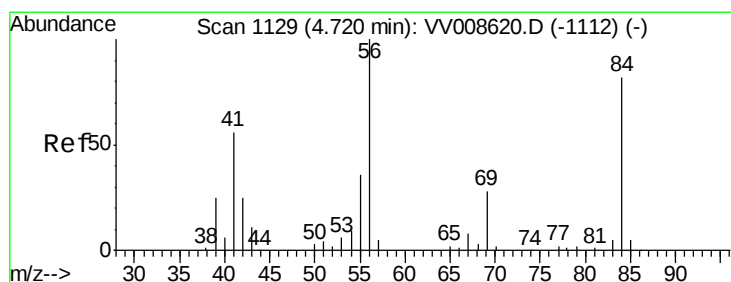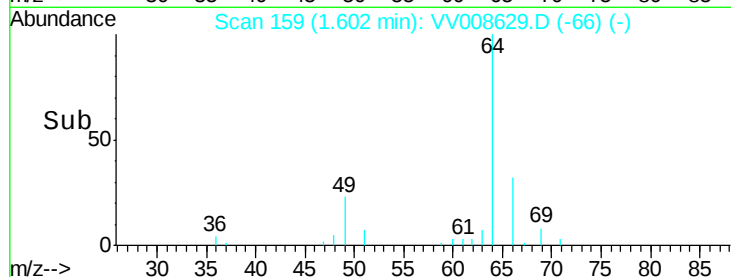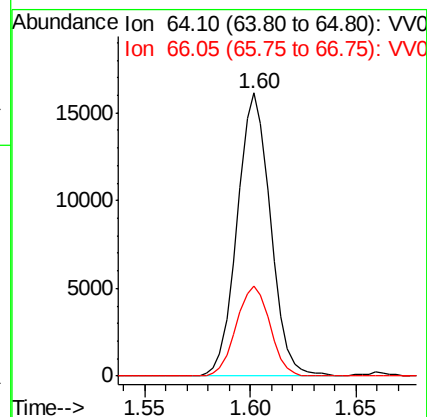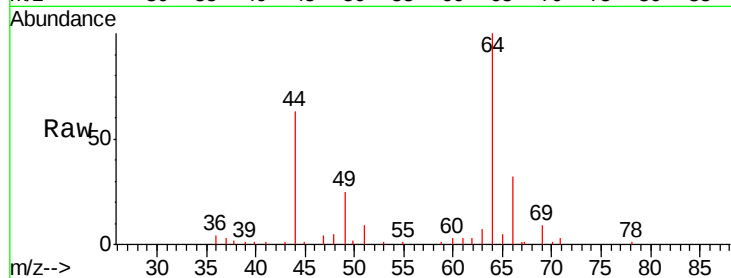

#30

Cyclohexane

Concen: 0.25 ug/L

RT: 4.73 min Scan# 1132

Delta R.T. 0.01 min

Lab File: VV008629.D

Acq: 17 Nov 2018 15:13




Tgt Ion: 56 Resp: 5010


Ion Ratio Lower Upper

56 100

69 28.7 24.2 36.4

84 83.8 65.7 98.5

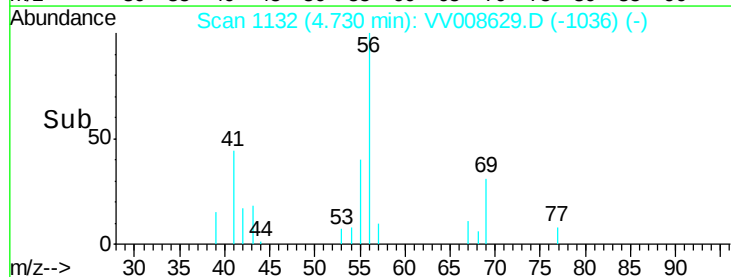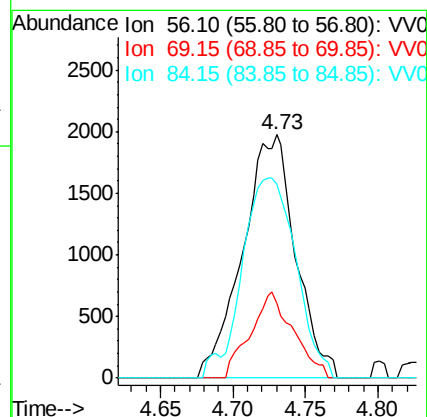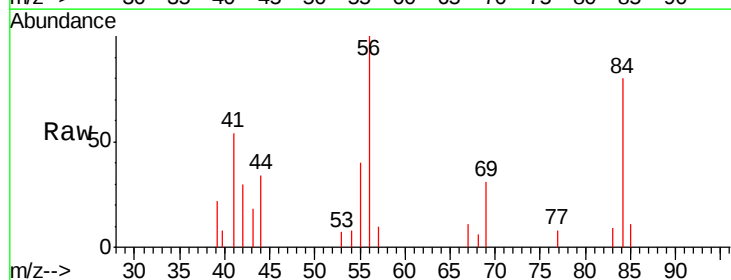

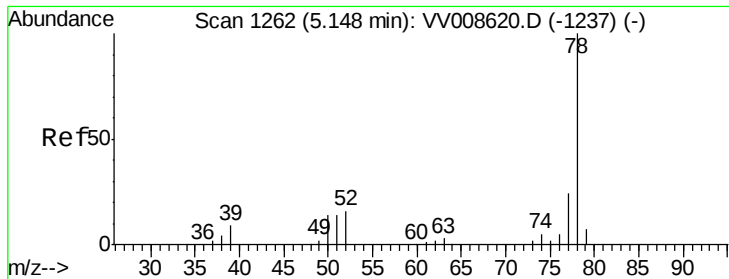

#33

Benzene

Concen: 2.90 ug/L

RT: 5.15 min Scan# 1263


Delta R.T. 0.00 min

Lab File: VV008629.D




Acq: 17 Nov 2018 15:13

Instrument :
MSVOA_V
ClientSampled :
ETO79

Tgt Ion: 78 Resp: 129635

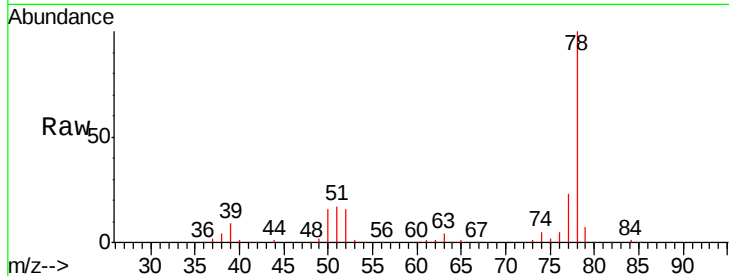

Abundance Ion 78.10 (77.80 to 78.80): VV0

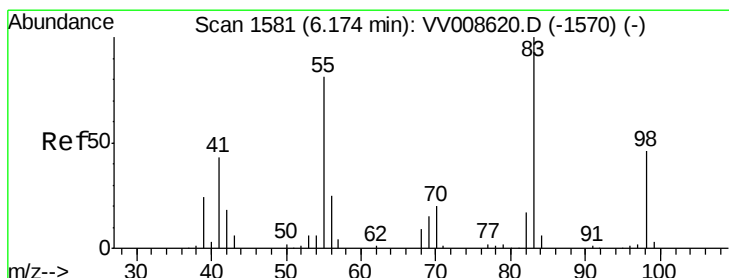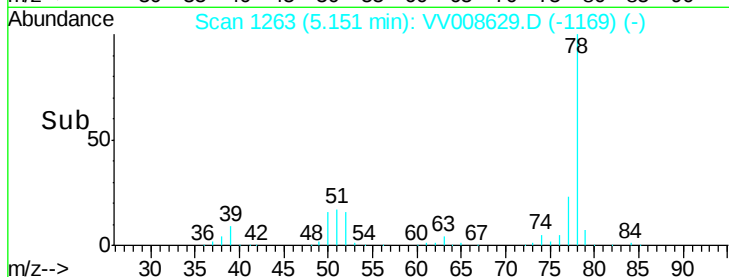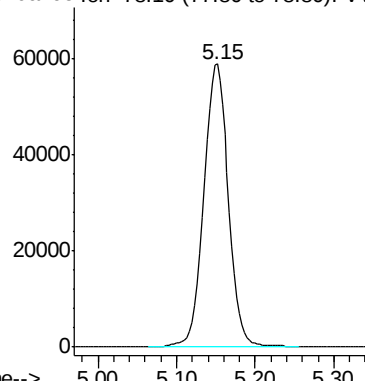

#35

Methylcyclohexane

Concen: 0.12 ug/L

RT: 6.18 min Scan# 1583


Delta R.T. 0.01 min

Lab File: VV008629.D

Acq: 17 Nov 2018 15:13



Tgt Ion: 83 Resp: 2371


Ion	Ratio	Lower	Upper
83	100		
55	104.6	65.6	98.4#
98	43.1	36.4	54.6

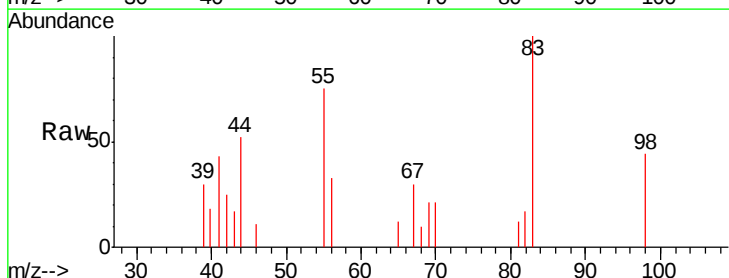

Abundance Ion 83.15 (82.85 to 83.85): VV0

Ion 55.10 (54.80 to 55.80): VV0
Ion 98.15 (97.85 to 98.85): VV0

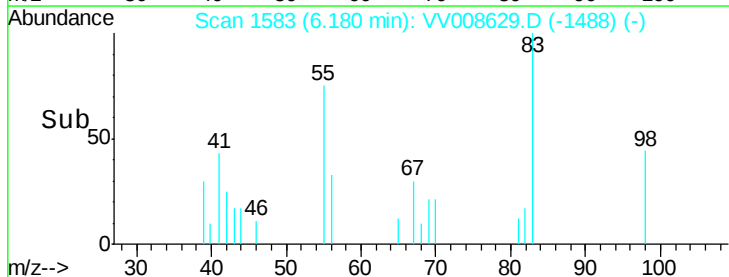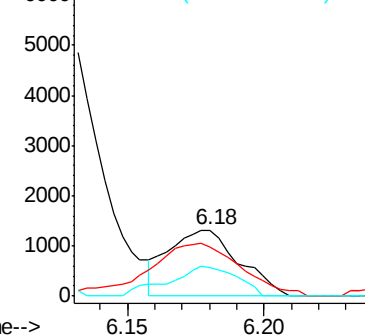

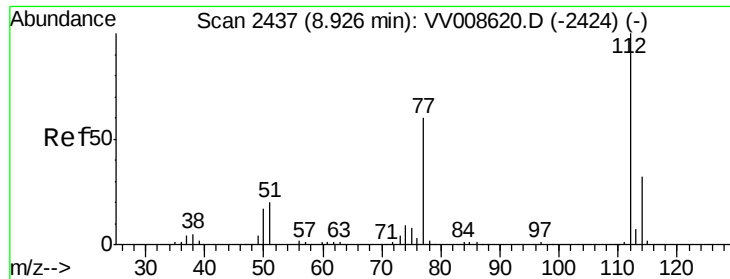

#51

Chlorobenzene

Concen: 3.69 ug/L

RT: 8.93 min Scan# 2437

Delta R.T. 0.00 min

Lab File: VV008629.D

Acq: 17 Nov 2018 15:13

Instrument :

MSVOA_V

ClientSampleId :

ETO79


Tgt Ion:112 Resp: 105782

Ion Ratio Lower Upper

112 100

114 31.9 21.9 40.7




77 59.7 47.9 71.9

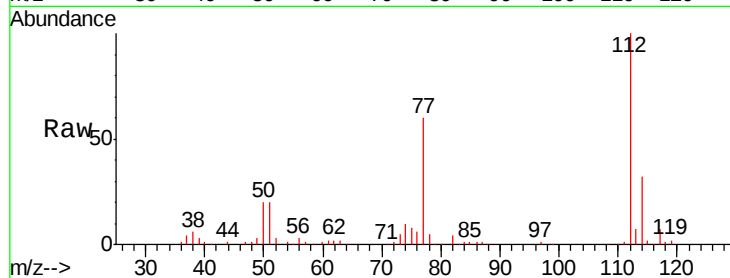

Abundance Ion 112.10 (111.80 to 112.80): V

Ion 114.05 (113.75 to 114.75): V

Ion 77.10 (76.80 to 77.80): VV0

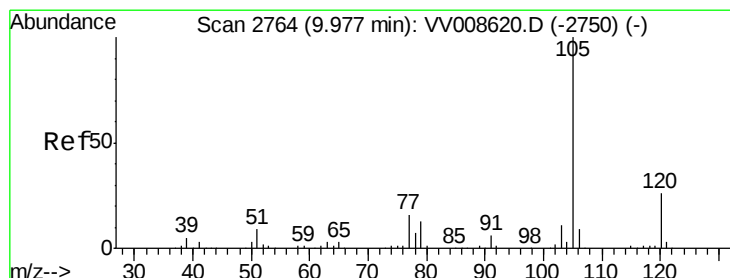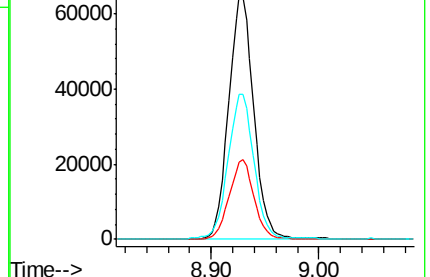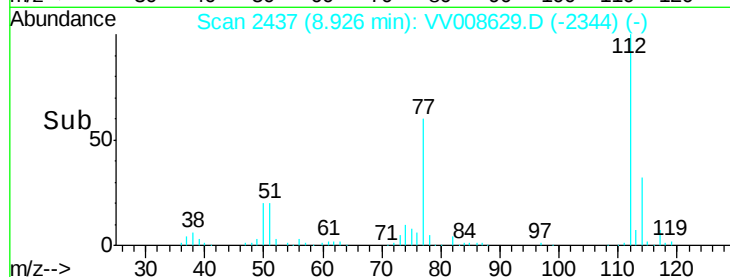

#56

Isopropylbenzene

Concen: 0.63 ug/L

RT: 9.98 min Scan# 2764

Delta R.T. 0.00 min

Lab File: VV008629.D

Acq: 17 Nov 2018 15:13


Tgt Ion:105 Resp: 31139

Ion Ratio Lower Upper

105 100

120 26.2 21.0 31.6



77 16.3 13.0 19.4

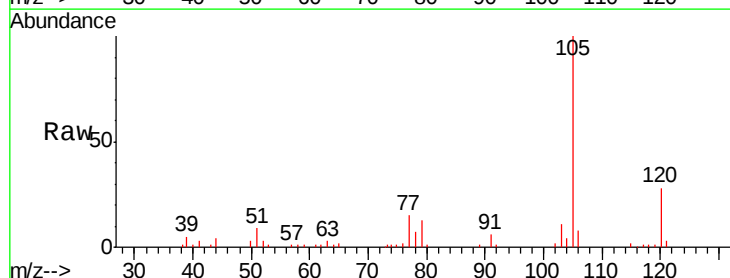


Abundance Ion 105.05 (104.75 to 105.75): V

Ion 120.10 (119.80 to 120.80): V

Ion 77.10 (76.80 to 77.80): VV0

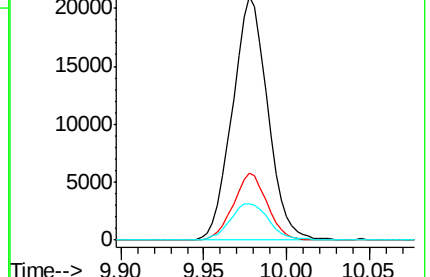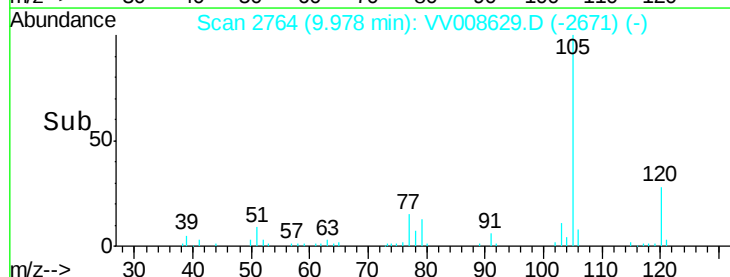

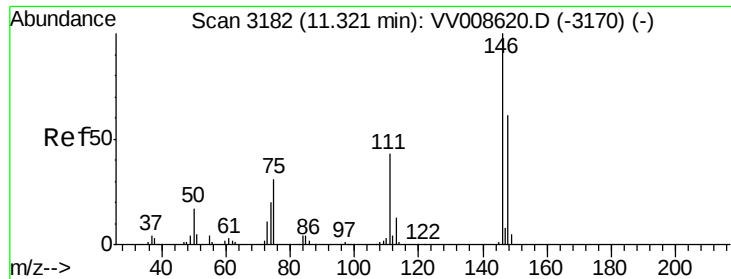

#63

1,4-Dichlorobenzene

Concen: 1.73 ug/L

RT: 11.32 min Scan# 3182

Delta R.T. 0.00 min

Lab File: VV008629.D

Acq: 17 Nov 2018 15:13

Instrument :

MSVOA_V

ClientSampleId :

ETO79


Tgt Ion:146 Resp: 34100

Ion Ratio Lower Upper

146 100

111 39.5 28.2 52.4




148 60.0 44.1 81.9

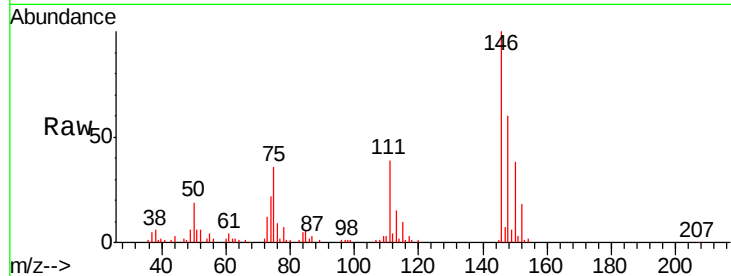

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

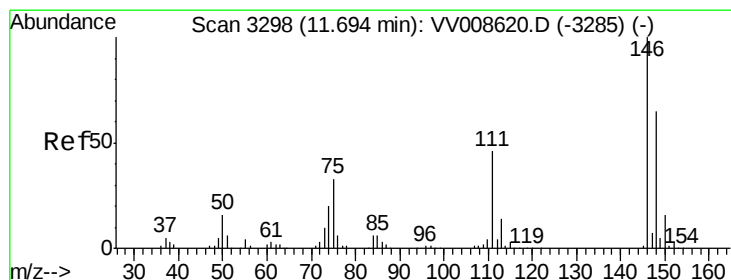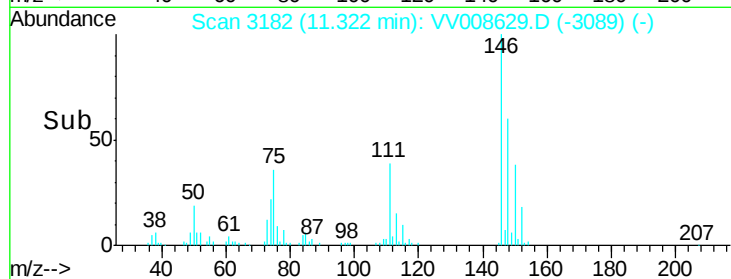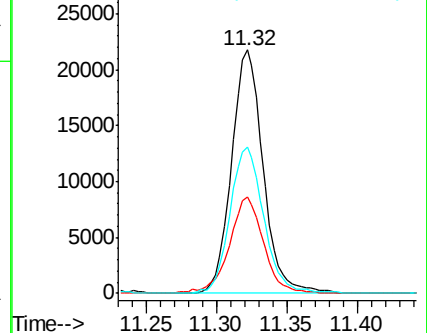

#65

1,2-Dichlorobenzene

Concen: 0.23 ug/L

RT: 11.69 min Scan# 3297

Delta R.T. -0.00 min

Lab File: VV008629.D

Acq: 17 Nov 2018 15:13


Tgt Ion:146 Resp: 4445

Ion Ratio Lower Upper

146 100

111 53.0 33.5 50.3#

148 72.2 50.0 75.0

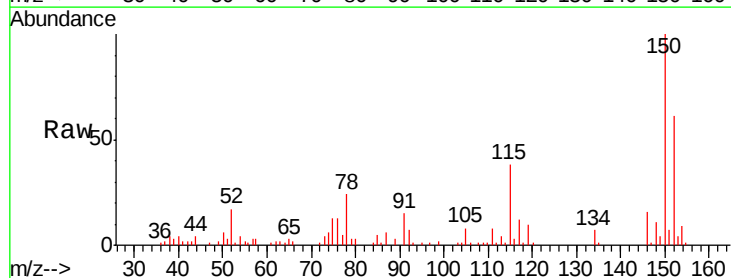

Abundance Ion 145.95 (145.65 to 146.65): V

Ion 111.00 (110.70 to 111.70): V

Ion 148.00 (147.70 to 148.70): V

