

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
 Data File : VV008630.D
 Acq On : 17 Nov 2018 15:38
 Operator : SY/MD
 Sample : J5990-06
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETO69

Quant Time: Nov 19 06:24:28 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 19 02:55:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	117430	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	105082	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	45686	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	23761	4.56	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.20%
7) Chloroethane-d5	1.59	69	18759	4.37	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	87.40%
11) 1,1-Dichloroethene-d2	2.14	63	36972	3.49	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	69.80%
20) 2-Butanone-d5	3.96	46	99368	53.24	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	106.48%
24) Chloroform-d	4.41	84	64873	4.55	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.00%
26) 1,2-Dichloroethane-d4	5.09	65	35714	4.92	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	98.40%
32) Benzene-d6	5.10	84	132648	4.84	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.80%
36) 1,2-Dichloropropane-d6	6.12	67	42963	4.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.20%
41) Toluene-d8	7.36	98	116550	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	90.60%
43) trans-1,3-Dichloropropene-	7.67	79	14181	4.21	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.20%
46) 2-Hexanone-d5	8.14	63	71704	46.95	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	93.90%
57) 1,1,2,2-Tetrachloroethane-	10.27	84	30046	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	11.67	152	40497	4.91	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	98.20%


Target Compounds					Qvalue
13) Acetone	2.21	43	6205	6.37 ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
Data File : VV008630.D
Acq On : 17 Nov 2018 15:38
Operator : SY/MD
Sample : J5990-06
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETO69

Quant Time: Nov 19 06:24:28 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 19 02:55:31 2018
Response via : Initial Calibration

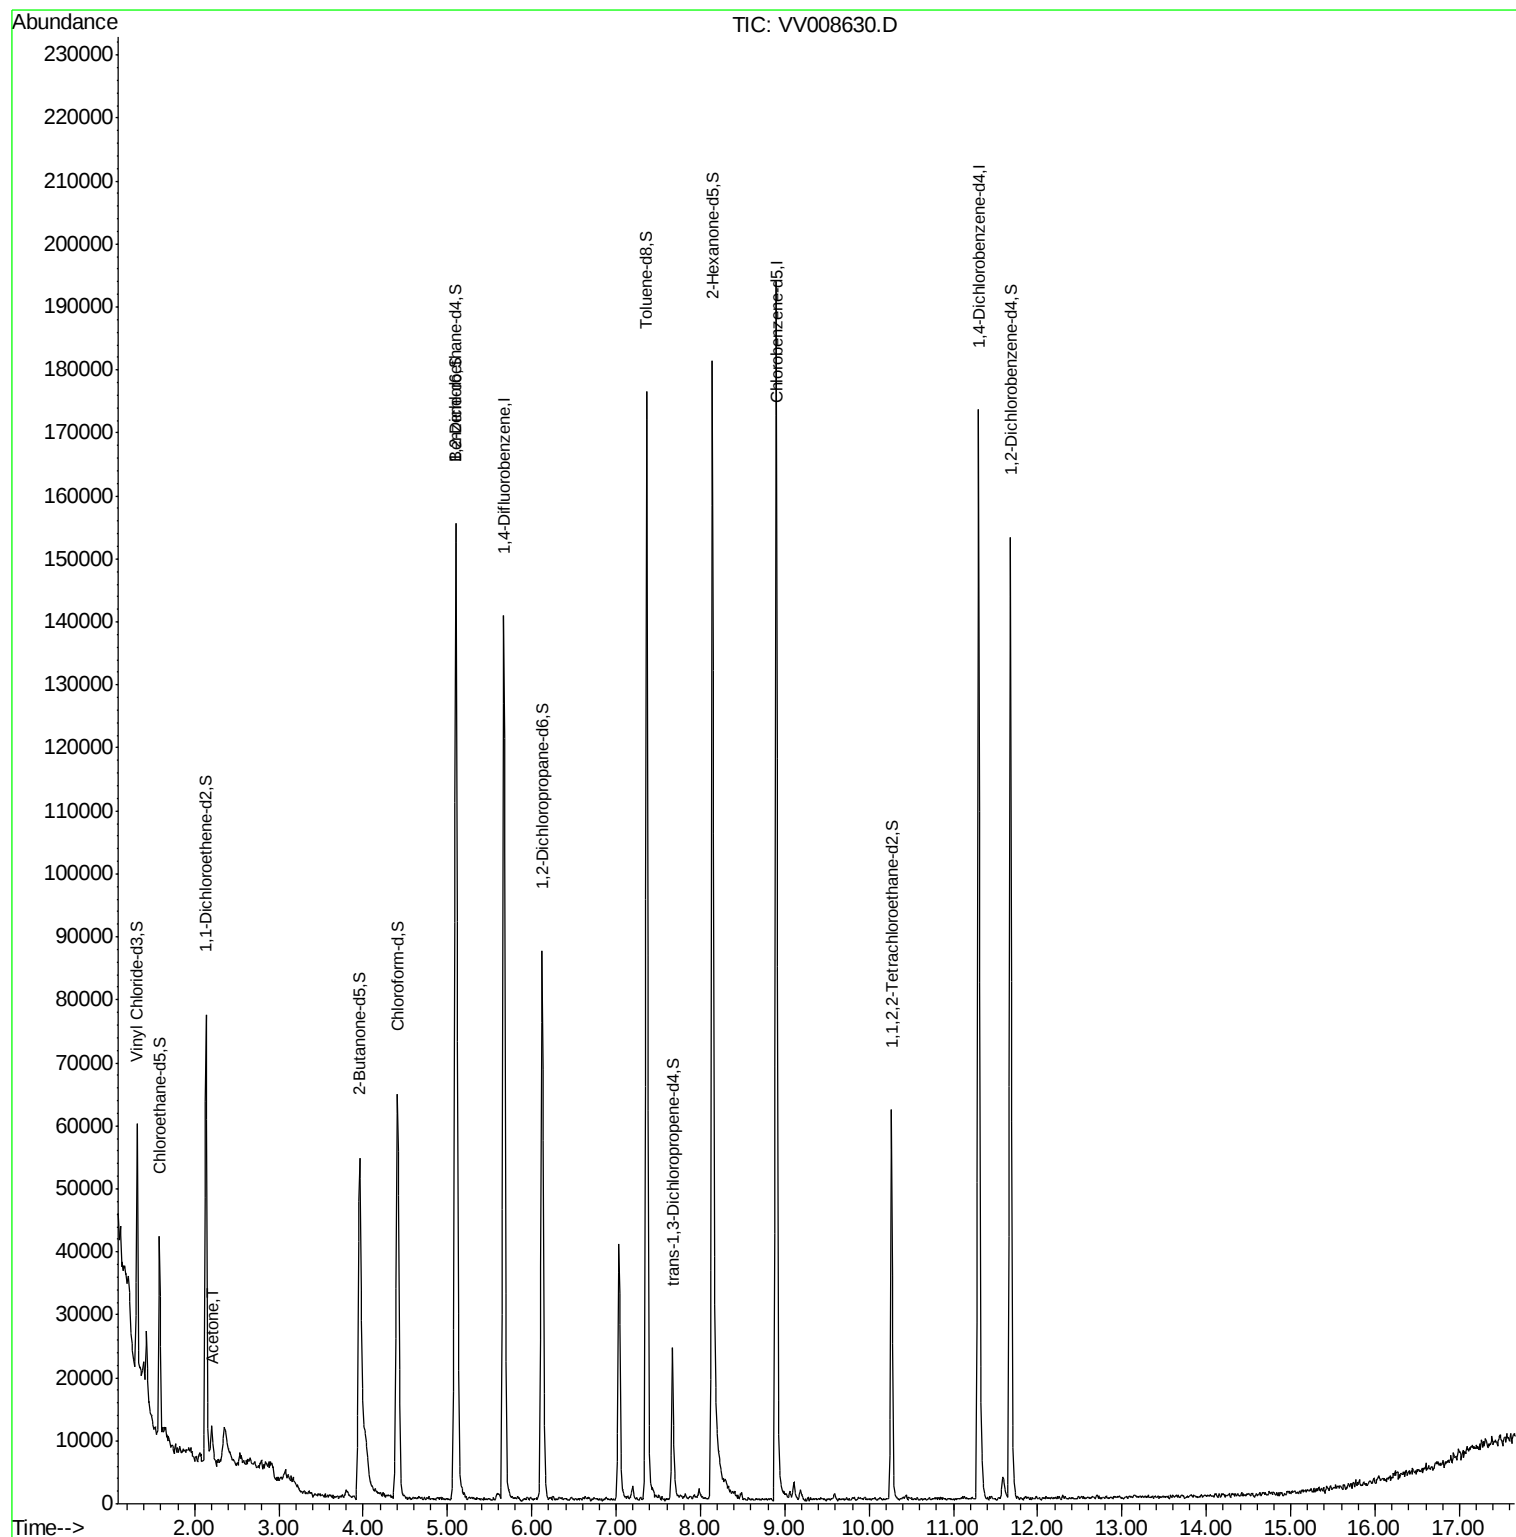

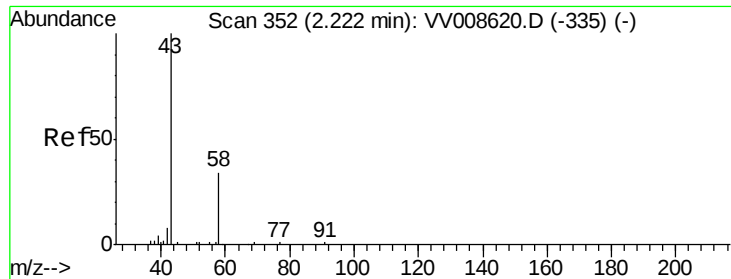

#13

Acetone

Concen: 6.37 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.02 min

Lab File: VV008630.D

Acq: 17 Nov 2018 15:38

Instrument :
MSVOA_V
ClientSampleId :
ETO69

Tgt Ion: 43 Resp: 6205

Ion Ratio Lower Upper

43 100

58 33.0 0.0 56.4

