

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
 Data File : VV008633.D
 Acq On : 17 Nov 2018 17:19
 Operator : SY/MD
 Sample : J5990-09
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETO72

Quant Time: Nov 19 06:49:19 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 19 02:55:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	129936	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	116417	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	51388	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	27486	4.76	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	95.20%
7) Chloroethane-d5	1.59	69	22366	4.71	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	94.20%
11) 1,1-Dichloroethene-d2	2.14	63	41298	3.53	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	70.60%
20) 2-Butanone-d5	3.96	46	105464	51.07	ug/L	-0.01
Spiked Amount	50.000	Range	40 - 130	Recovery	=	102.14%
24) Chloroform-d	4.41	84	71424	4.53	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	90.60%
26) 1,2-Dichloroethane-d4	5.09	65	38827	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	96.60%
32) Benzene-d6	5.10	84	146726	4.83	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	96.60%
36) 1,2-Dichloropropane-d6	6.12	67	46156	4.71	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	94.20%
41) Toluene-d8	7.36	98	133262	4.67	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	93.40%
43) trans-1,3-Dichloropropene-	7.67	79	15777	4.22	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	84.40%
46) 2-Hexanone-d5	8.14	63	76841	45.42	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.84%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	31746	4.64	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	92.80%
64) 1,2-Dichlorobenzene-d4	11.68	152	44752	4.82	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	96.40%


Target Compounds					Qvalue
13) Acetone	2.20	43	4525	4.20 ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
Data File : VV008633.D
Acq On : 17 Nov 2018 17:19
Operator : SY/MD
Sample : J5990-09
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETO72

Quant Time: Nov 19 06:49:19 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 19 02:55:31 2018
Response via : Initial Calibration

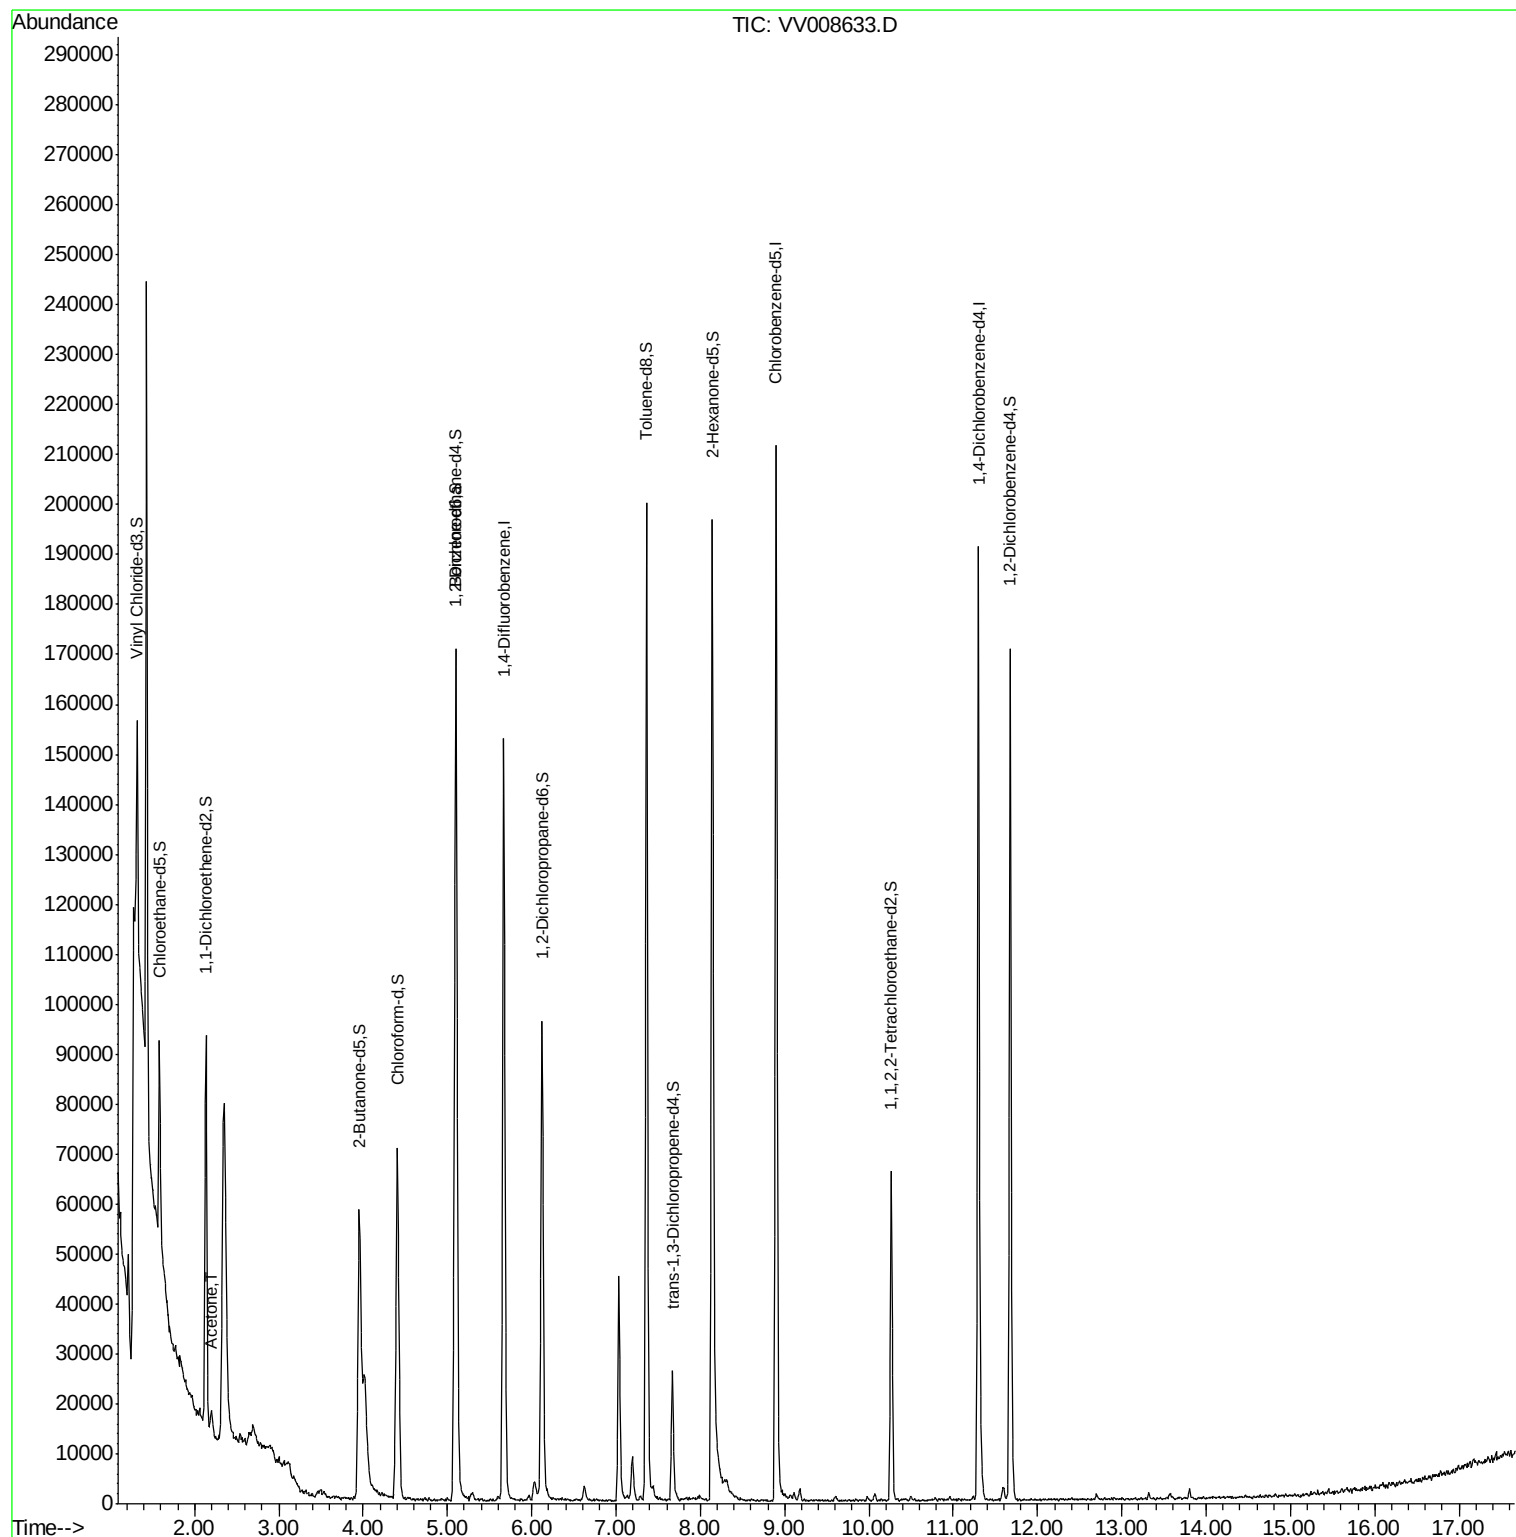

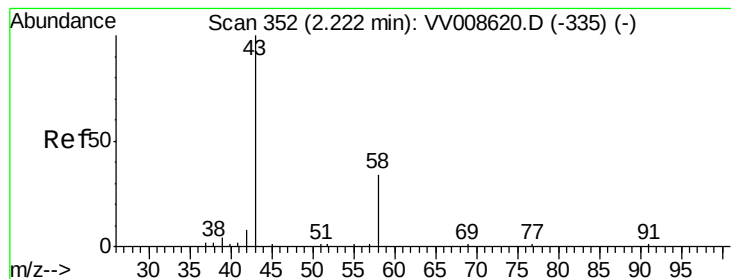

#13

Acetone

Concen: 4.20 ug/L

RT: 2.20 min Scan# 346

Delta R.T. -0.02 min

Lab File: VV008633.D

Acq: 17 Nov 2018 17:19

Instrument :
MSVOA_V
ClientSampleId :
ETO72

Tgt Ion: 43 Resp: 4525

Ion Ratio Lower Upper

43 100

58 32.2 0.0 56.4

