

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
 Data File : VV008635.D
 Acq On : 17 Nov 2018 18:09
 Operator : SY/MD
 Sample : J5990-11
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETO71

Quant Time: Nov 19 07:53:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 19 02:55:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	127969	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	113826	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	49816	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	25972	4.57	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	91.40%
7) Chloroethane-d5	1.59	69	21461	4.59	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	91.80%
11) 1,1-Dichloroethene-d2	2.14	63	39656	3.44	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	68.80%
20) 2-Butanone-d5	3.96	46	102814	50.55	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	101.10%
24) Chloroform-d	4.41	84	70907	4.57	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	91.40%
26) 1,2-Dichloroethane-d4	5.09	65	38600	4.88	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	97.60%
32) Benzene-d6	5.10	84	143958	4.85	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	97.00%
36) 1,2-Dichloropropane-d6	6.12	67	46576	4.86	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.20%
41) Toluene-d8	7.36	98	128732	4.62	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	92.40%
43) trans-1,3-Dichloropropene-	7.67	79	14395	3.94	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	78.80%
46) 2-Hexanone-d5	8.14	63	73574	44.47	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	88.94%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	32095	4.80	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	96.00%
64) 1,2-Dichlorobenzene-d4	11.68	152	43876	4.88	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	97.60%


Target Compounds					Qvalue
13) Acetone	2.20	43	5721	5.39 ug/L	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
Data File : VV008635.D
Acq On : 17 Nov 2018 18:09
Operator : SY/MD
Sample : J5990-11
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETO71

Quant Time: Nov 19 07:53:16 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 19 02:55:31 2018
Response via : Initial Calibration

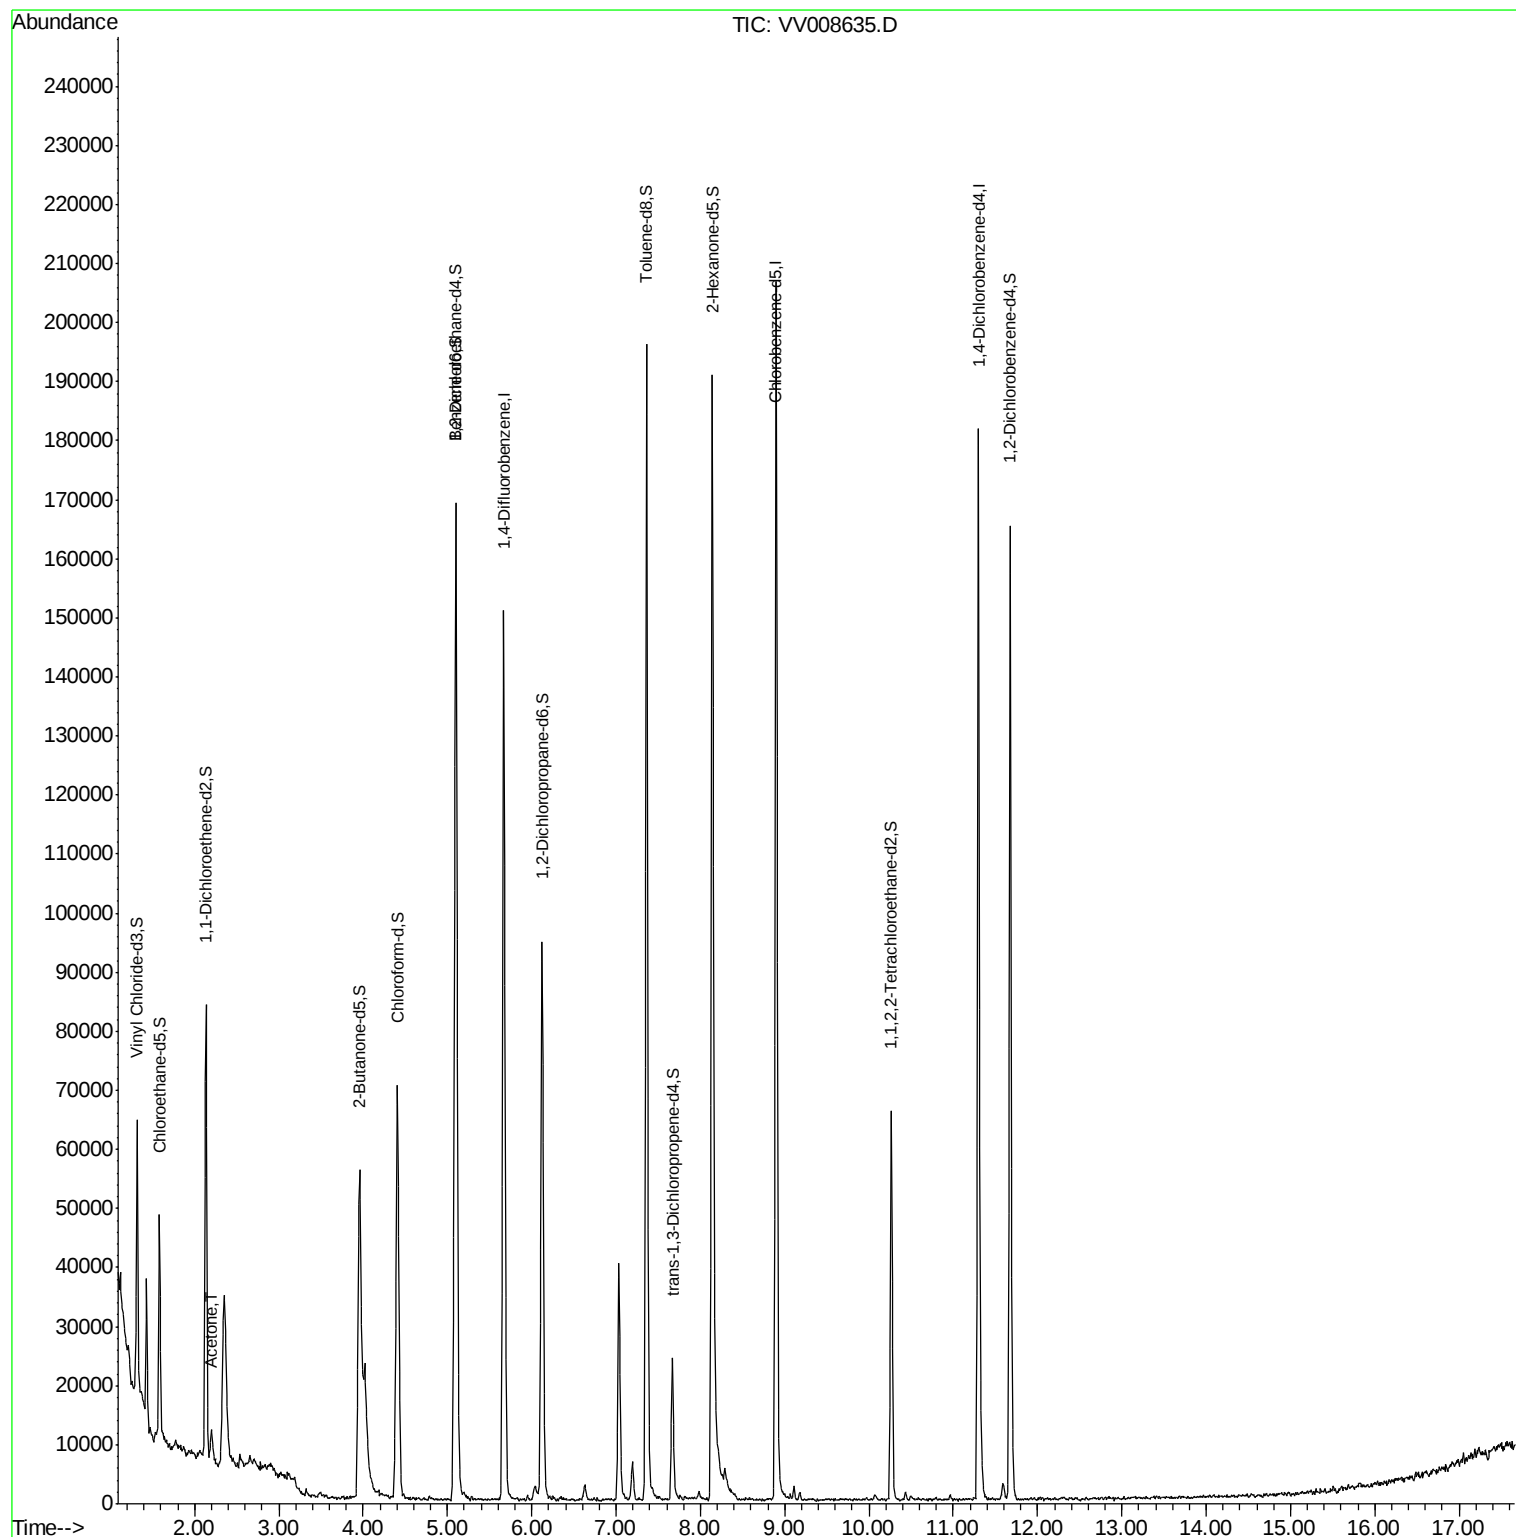

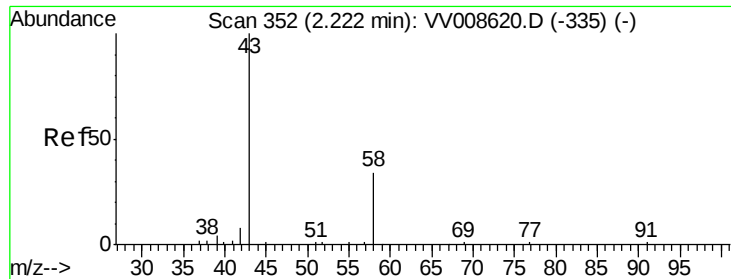

#13

Acetone

Concen: 5.39 ug/L

RT: 2.20 min Scan# 346

Delta R.T. -0.02 min

Lab File: VV008635.D

Acq: 17 Nov 2018 18:09

Instrument :
MSVOA_V
ClientSampleId :
ETO71

Tgt Ion: 43 Resp: 5721

Ion Ratio Lower Upper

43 100

58 33.4 0.0 56.4

