

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
 Data File : VV008636.D
 Acq On : 17 Nov 2018 18:34
 Operator : SY/MD
 Sample : J5990-12
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 ETO75

Quant Time: Nov 19 08:12:35 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Mon Nov 19 02:55:31 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.67	114	124431	5.00	ug/L	0.00
28) Chlorobenzene-d5	8.90	117	111869	5.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	11.30	152	49470	5.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	1.32	65	25085	4.54	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	90.80%
7) Chloroethane-d5	1.59	69	22490	4.94	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	98.80%
11) 1,1-Dichloroethene-d2	2.14	63	35952	3.21	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	64.20%
20) 2-Butanone-d5	3.96	46	104732	52.96	ug/L	-0.02
Spiked Amount	50.000	Range	40 - 130	Recovery	=	105.92%
24) Chloroform-d	4.41	84	70953	4.70	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	94.00%
26) 1,2-Dichloroethane-d4	5.09	65	39804	5.17	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	103.40%
32) Benzene-d6	5.10	84	147969	5.07	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	101.40%
36) 1,2-Dichloropropane-d6	6.12	67	46061	4.89	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	97.80%
41) Toluene-d8	7.36	98	129629	4.73	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	94.60%
43) trans-1,3-Dichloropropene-	7.67	79	14430	4.02	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	80.40%
46) 2-Hexanone-d5	8.14	63	73467	45.19	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	90.38%
57) 1,1,2,2-Tetrachloroethane-	10.26	84	31950	4.86	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	97.20%
64) 1,2-Dichlorobenzene-d4	11.68	152	45212	5.06	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	101.20%


Target Compounds					Qvalue
13) Acetone	2.21	43	5660	5.49 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
Data File : VV008636.D
Acq On : 17 Nov 2018 18:34
Operator : SY/MD
Sample : J5990-12
Misc : 25.0 mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
ETO75

Quant Time: Nov 19 08:12:35 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Mon Nov 19 02:55:31 2018
Response via : Initial Calibration

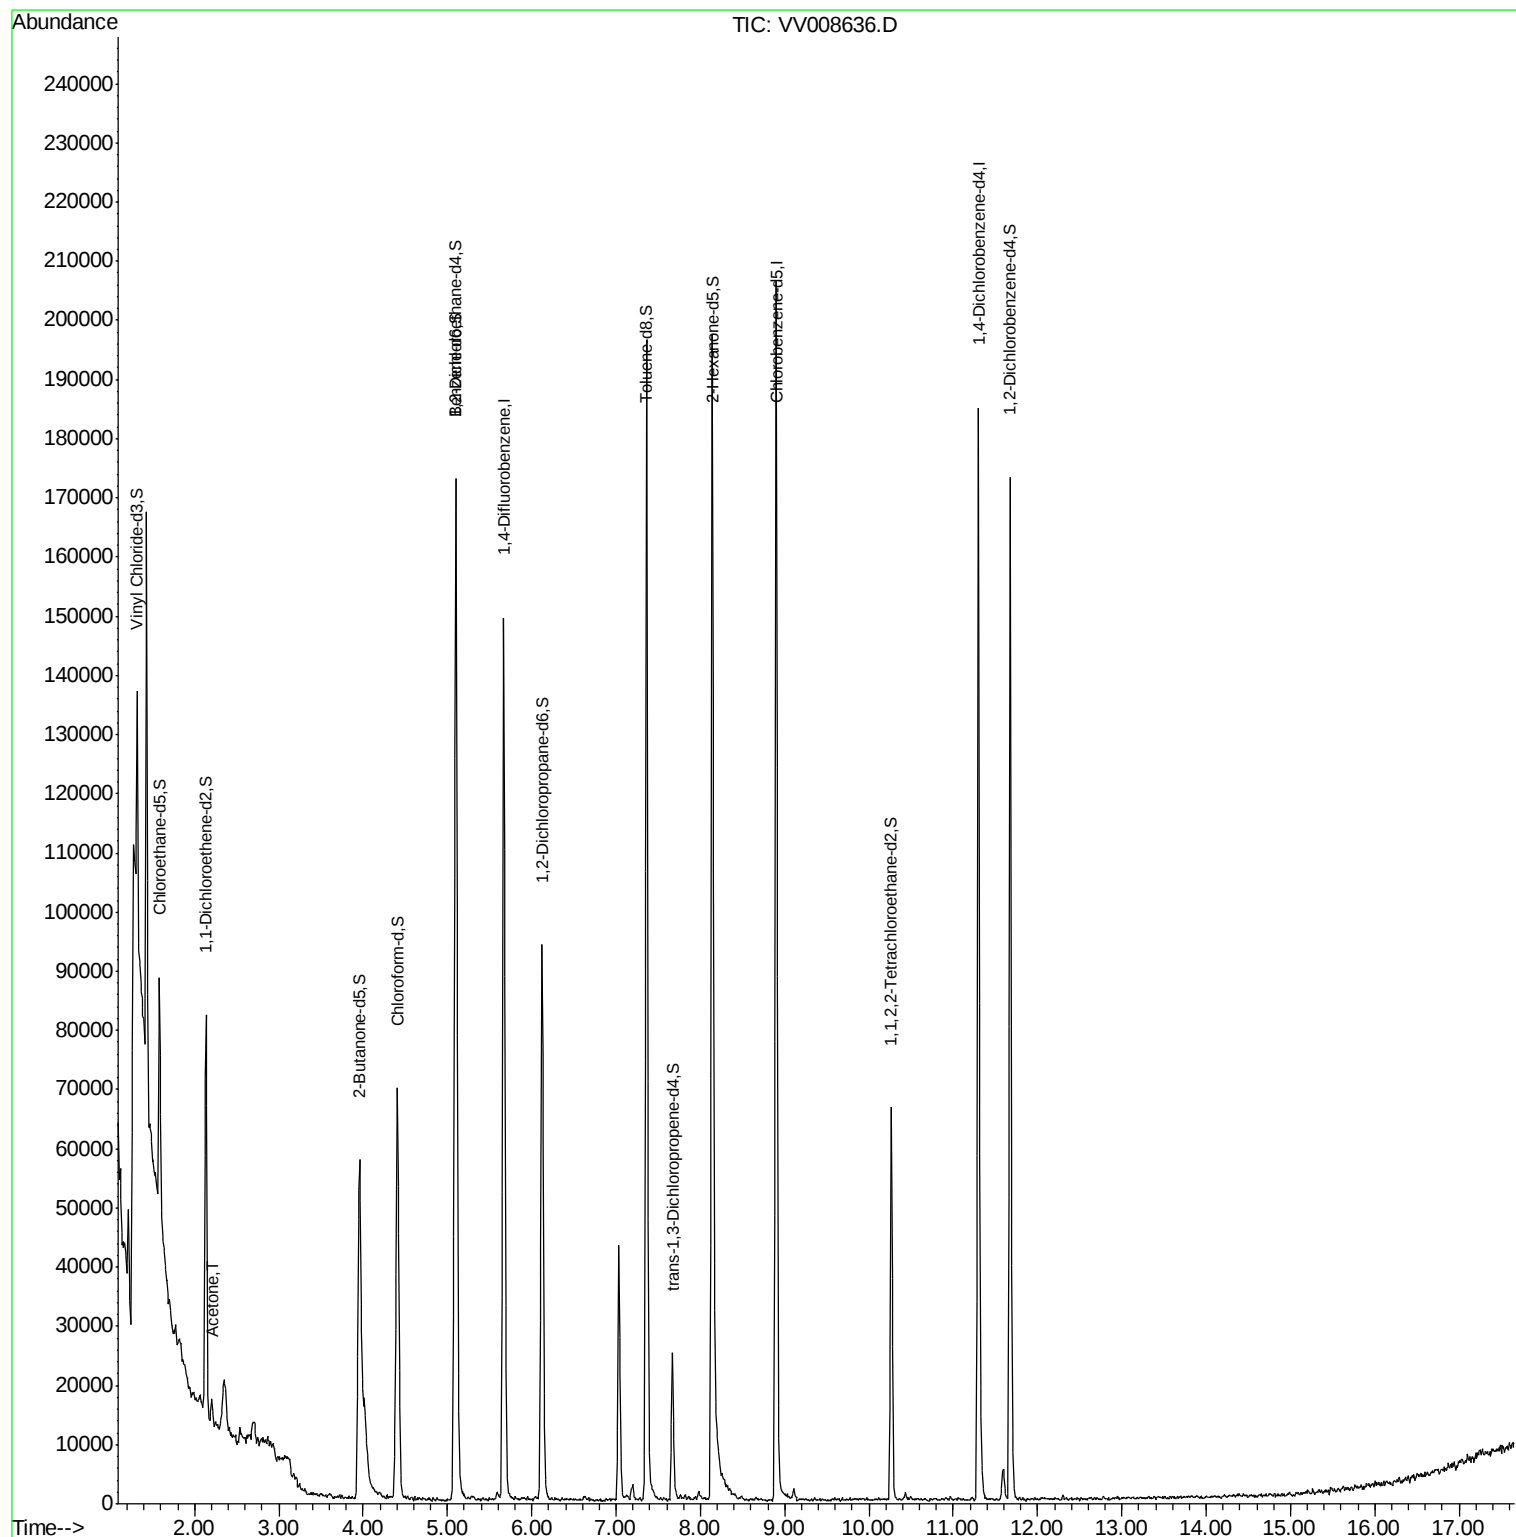

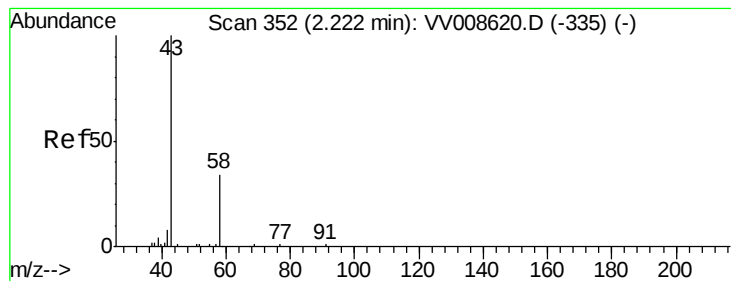

#13

Acetone

Concen: 5.49 ug/L

RT: 2.21 min Scan# 347

Delta R.T. -0.02 min

Lab File: VV008636.D

Acq: 17 Nov 2018 18:34

Instrument :
MSVOA_V
ClientSampleId :
ETO75

Tgt Ion: 43 Resp: 5660

Ion Ratio Lower Upper

43 100

58 27.2 0.0 56.4

