


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_V\DATA\VV111818\
 Data File : VV008619.D
 Acq On : 17 Nov 2018 09:21
 Operator : SY/MD
 Sample : BFB49
 Misc : 25.0 mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB49

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111718WMA.M
 Title : TRACE VOA SOM01.0
 Last Update : Mon Nov 19 02:55:31 2018

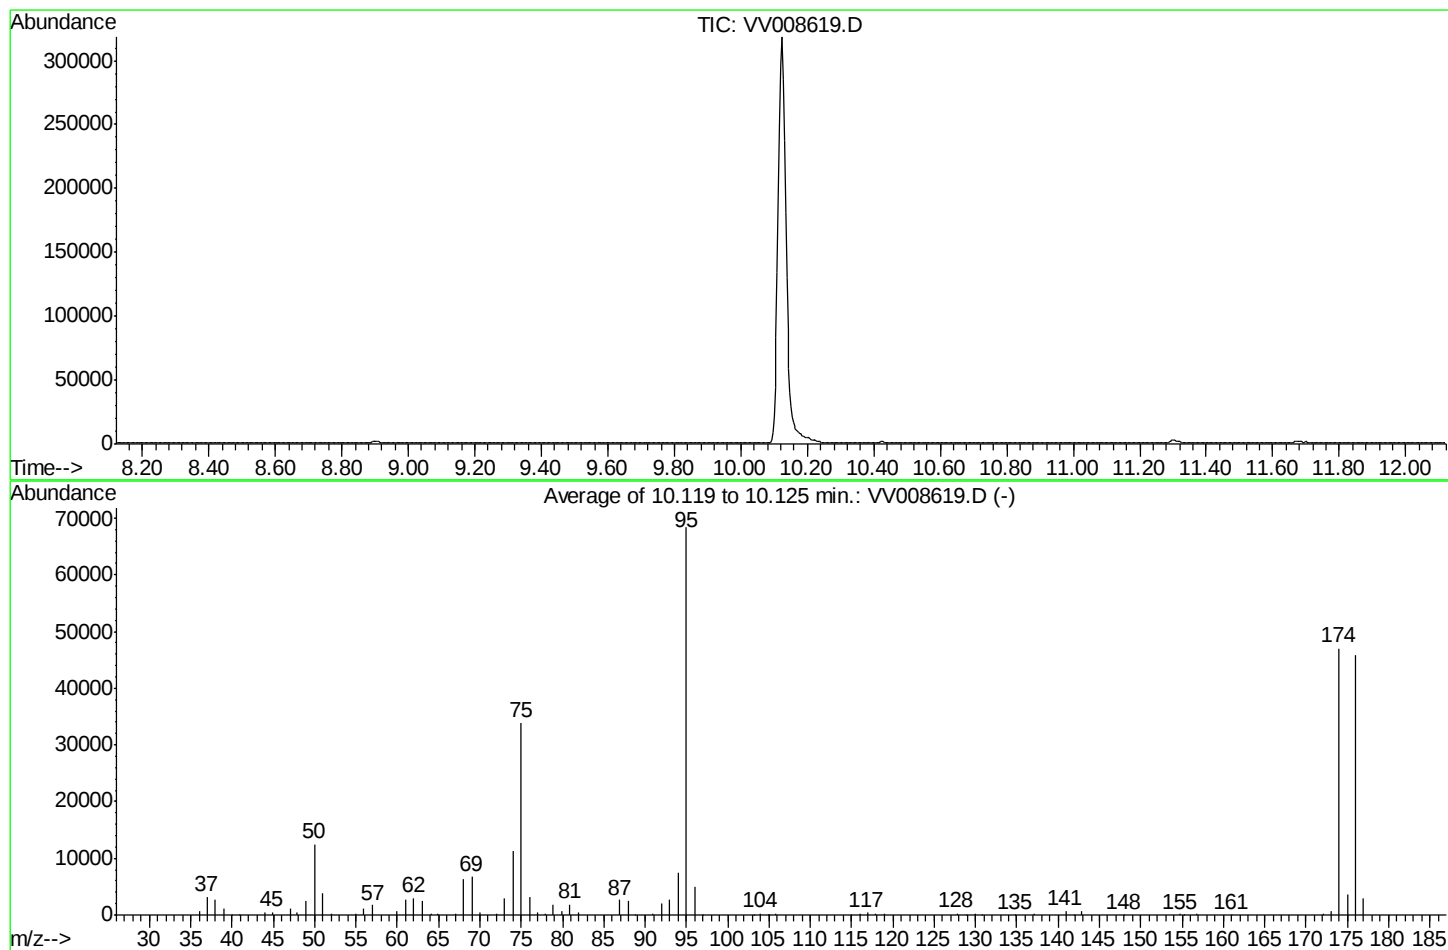

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.3	12501	PASS
75	95	30	80	49.6	33880	PASS
95	95	100	100	100.0	68373	PASS
96	95	5	9	7.2	4911	PASS
173	174	0.00	2	1.6	762	PASS
174	95	50	120	68.8	47066	PASS
175	174	5	9	7.8	3679	PASS
176	174	95	101	97.5	45890	PASS
177	176	5	9	6.5	2988	PASS

m/z	Abundance
36.00	650.0
37.00	3133.0
38.00	2628.0
39.00	1151.0
40.00	231.0
40.90	123.0
43.90	821.0
44.90	548.0
47.00	1048.0
47.80	367.0
49.00	2355.0
50.00	12176.0
51.00	3775.0
52.00	205.0
55.00	163.0
56.00	1011.0
57.00	1660.0
59.90	568.0
61.00	2699.0
62.00	2808.0
63.00	2326.0
64.00	229.0
64.90	283.0
67.00	252.0
68.00	6198.0
69.00	6392.0
70.10	562.0
71.90	310.0
73.00	2754.0
74.00	10694.0
75.00	32480.0
76.00	3109.0
77.00	447.0
77.90	275.0
78.90	1767.0
79.90	503.0
80.90	1857.0
81.90	404.0
87.00	2373.0
87.90	2274.0
88.70	131.0
90.90	219.0
92.00	1993.0
92.90	2657.0
94.00	7521.0
95.00	65752.0
96.00	4794.0
97.00	101.0
103.10	110.0
103.90	271.0
104.80	122.0
105.80	227.0
115.00	103.0
115.90	209.0
116.90	356.0
117.90	285.0
118.90	267.0
127.80	221.0
128.90	113.0
130.00	208.0
134.80	108.0
137.10	119.0
140.90	764.0
141.90	104.0
142.90	696.0
148.00	126.0
154.80	158.0
156.90	126.0
172.10	280.0
173.00	736.0
174.00	44056.0
175.00	3424.0
176.00	43320.0
177.00	2821.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

Scan 2796 (10.080 min): VV008619.D
BFB49

m/z	Abundance
39.90	213.0
43.90	522.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	772.0
37.00	3208.0
38.00	2597.0
39.00	1113.0
40.00	332.0
44.00	924.0
44.90	580.0
47.00	1000.0
47.90	439.0
49.00	2636.0
50.00	12482.0
51.00	3749.0
52.00	238.0
54.90	252.0
55.90	1071.0
57.00	1724.0
59.90	623.0
61.00	2869.0
61.90	3128.0
63.00	2423.0
64.00	341.0
65.00	263.0
67.00	292.0
68.00	6370.0
69.00	6856.0
70.00	482.0
72.00	281.0
73.00	3097.0
74.00	11629.0
75.00	34264.0
76.00	2913.0
77.00	377.0
77.90	292.0
78.90	1959.0
79.90	693.0
80.90	1867.0
81.90	385.0
86.90	2874.0
88.00	2435.0
91.00	242.0
92.00	2192.0
93.00	2870.0
94.00	7377.0
95.00	69048.0
96.00	4807.0
97.00	123.0
104.00	264.0
105.00	103.0
105.70	259.0
116.00	316.0
116.90	450.0
117.90	280.0
118.90	352.0
127.70	278.0
129.90	251.0
130.80	142.0
137.10	132.0
140.90	781.0
142.90	741.0
154.80	161.0
155.20	126.0
156.80	172.0
161.00	128.0
172.10	343.0
173.00	762.0
174.00	48768.0
175.00	3867.0
176.00	47144.0
177.00	3102.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49

m/z	Abundance
36.00	761.0
37.00	3355.0
38.00	2658.0
39.00	1193.0
40.00	281.0
40.90	116.0
44.00	905.0
44.90	545.0
47.00	1132.0
47.90	418.0
49.00	2610.0
50.00	12845.0
51.00	3924.0
52.00	217.0
54.90	222.0
55.90	1034.0
57.00	1753.0
59.90	636.0
61.00	2866.0
61.90	3161.0
63.00	2485.0
64.10	315.0
65.00	300.0
67.00	303.0
68.00	6470.0
69.00	7007.0
70.00	510.0
72.00	312.0
73.00	3035.0
74.00	11637.0
75.00	34896.0
76.00	3216.0
77.00	423.0
77.90	305.0
78.90	1976.0
79.90	630.0
80.90	1929.0
81.90	416.0
87.00	2736.0
87.90	2494.0
91.00	266.0
92.00	2149.0
92.90	2934.0
94.00	7687.0
95.00	70320.0
96.00	5133.0
103.90	278.0
105.70	252.0
116.00	274.0
116.90	431.0
118.00	303.0
118.90	287.0
127.70	263.0
129.90	239.0
130.70	104.0
137.10	151.0
140.90	825.0
142.90	755.0
148.00	101.0
154.80	157.0
156.90	152.0
172.10	338.0
173.00	788.0
174.00	48376.0
175.00	3746.0
176.00	47208.0
177.00	3041.0

Instrument :
MSVOA_V
ClientSampleId :
BFB49