
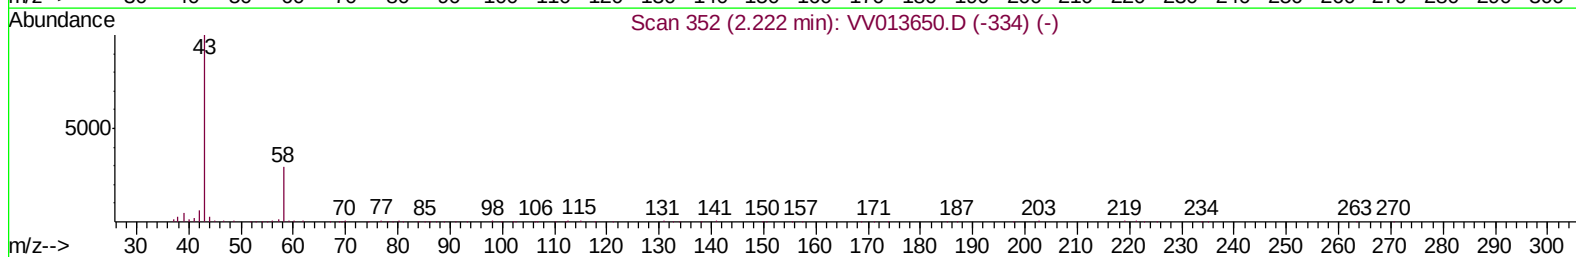
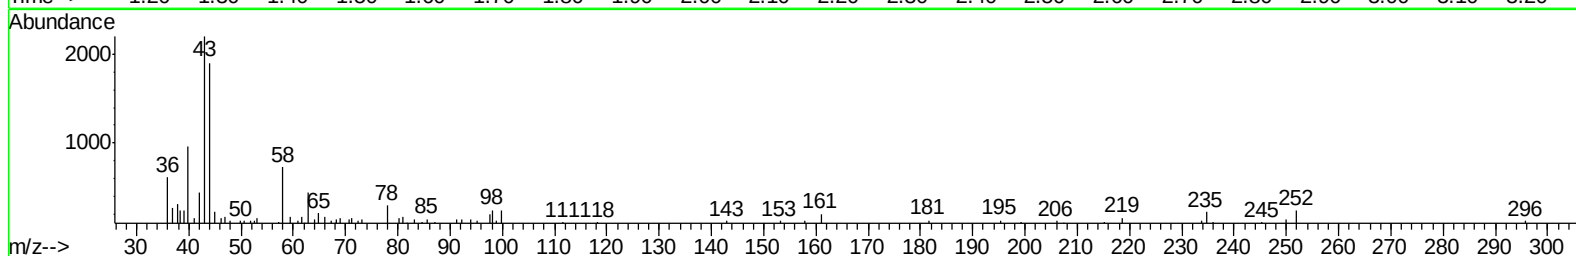


Data File : VV013656.D
Acq On : 18 Nov 2019 13:52
Operator : SY/MD
Sample : K5856-22
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Nov 19 04:28:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 19 04:25:23 2019
Response via : Initial Calibration

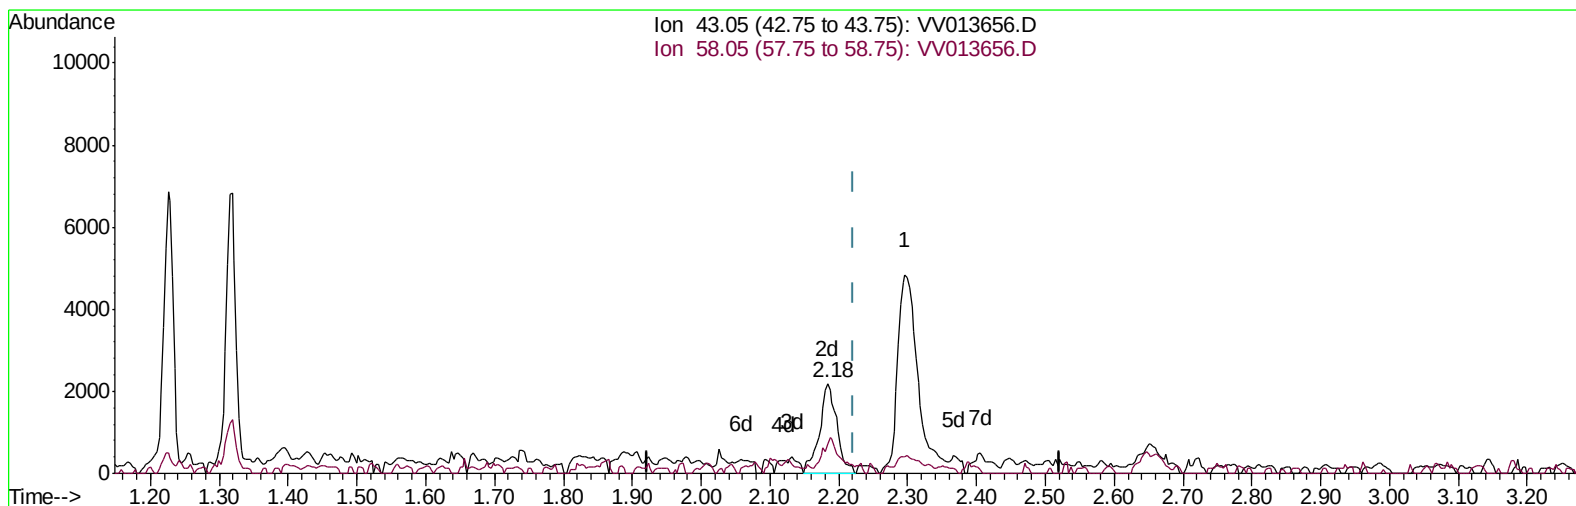

TIC: VV013656.D

(13) Acetone (T)

2.184min (-0.038) 1.30ug/L m

response 3827

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	27.15#
0.00	0.00	0.00
0.00	0.00	0.00