
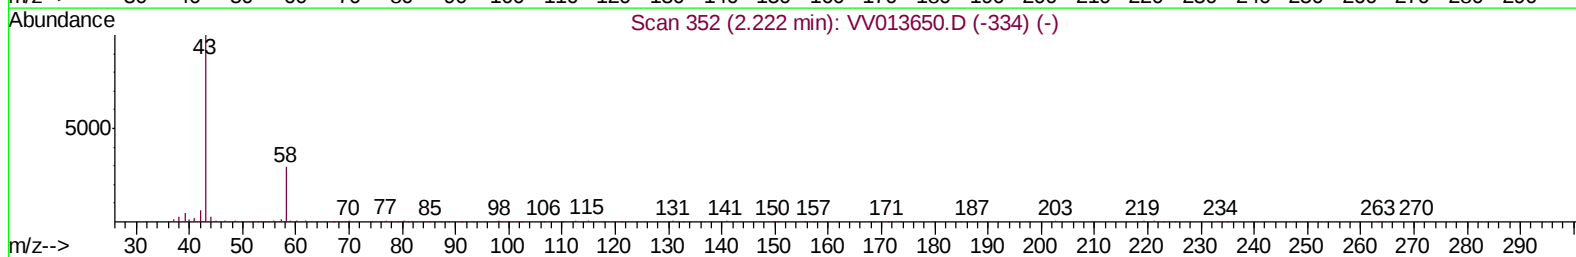
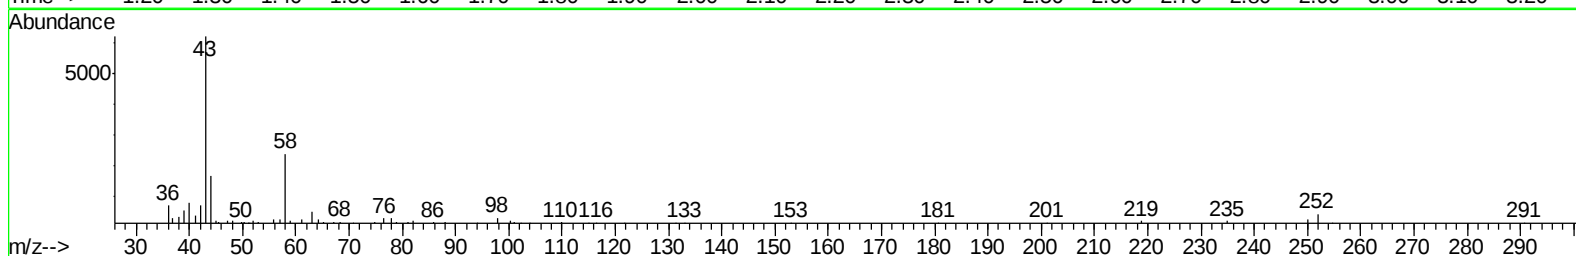


Data File : VV013657.D
Acq On : 18 Nov 2019 14:16
Operator : SY/MD
Sample : K5856-23
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Quant Time: Nov 19 04:28:46 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Tue Nov 19 04:25:23 2019
Response via : Initial Calibration

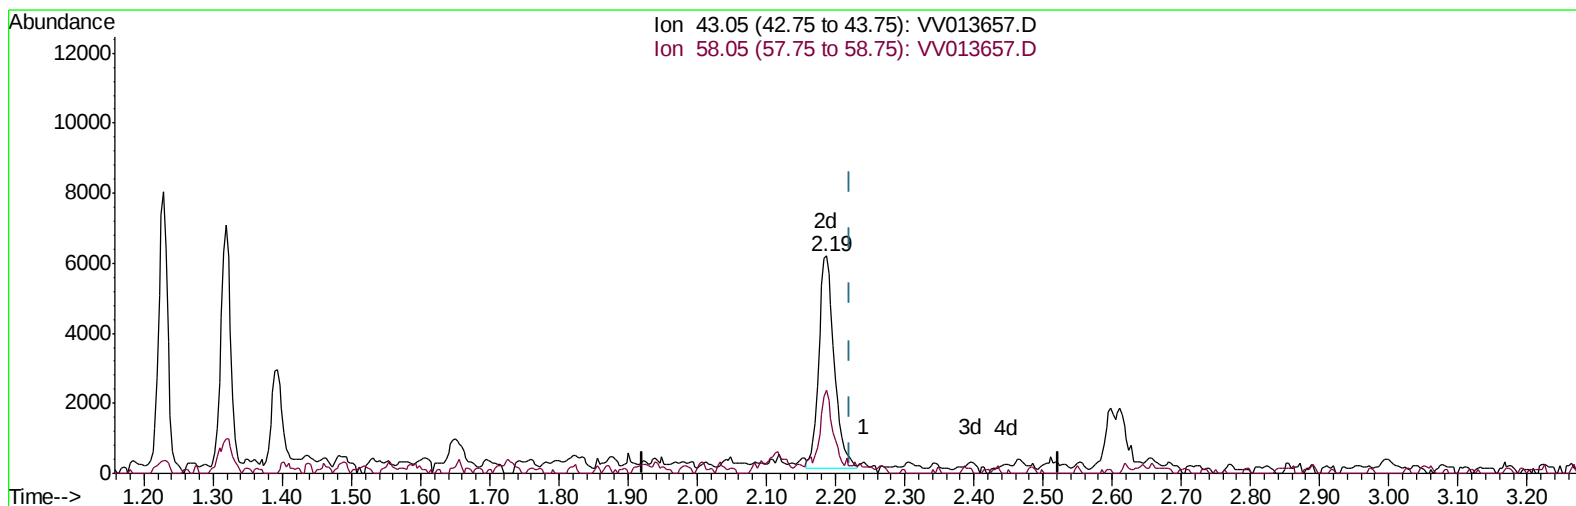

TIC: VV013657.D

(13) Acetone (T)

2.187min (-0.035) 2.79ug/L m

response 9300

Ion	Exp%	Act%
43.05	100	100
58.05	8.50	1.84
0.00	0.00	0.00
0.00	0.00	0.00