


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV111819\
Data File : VV013649.D
Acq On : 18 Nov 2019 10:13
Operator : SY/MD
Sample : BFB33
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB33

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SOMVTR111519WMA.M
Title : TRACE VOA SOM01.0
Last Update : Wed Nov 20 01:31:47 2019

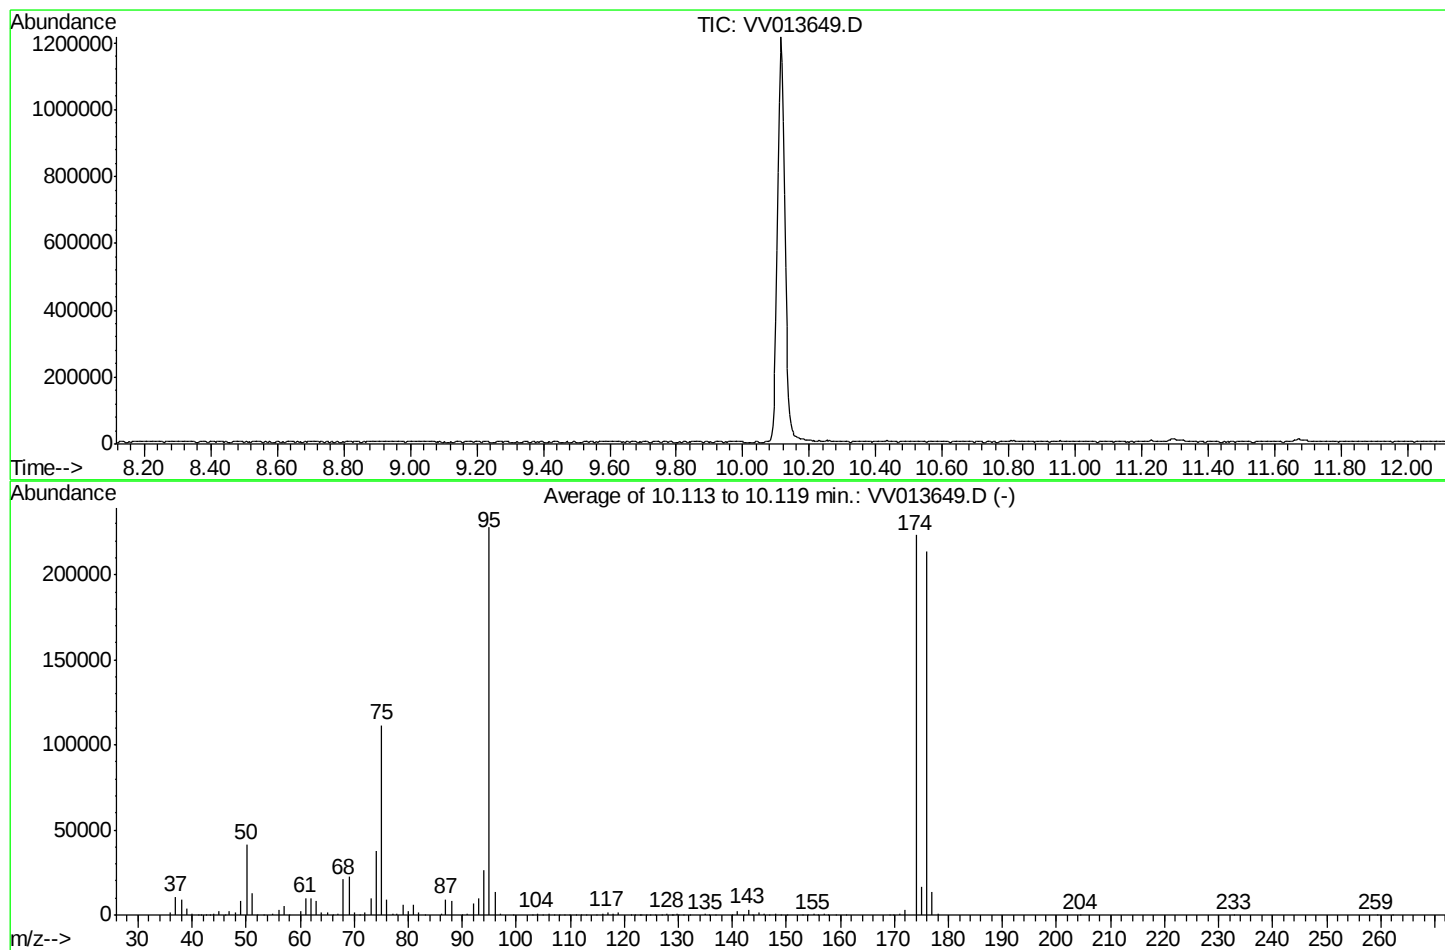

AutoFind: Scans 2806, 2807, 2808; Background Corrected with Scan 2792

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.1	41357	PASS
75	95	30	80	48.9	111421	PASS
95	95	100	100	100.0	227904	PASS
96	95	5	9	5.9	13521	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	98.0	223381	PASS
175	174	5	9	7.3	16397	PASS
176	174	95	101	95.7	213781	PASS
177	176	5	9	6.5	13944	PASS

m/z	Abundance
36.00	1910.0
37.00	10391.0
38.10	9511.0
39.00	4105.0
40.00	1296.0
41.20	171.0
41.70	181.0
42.70	185.0
43.20	262.0
44.00	1712.0
45.00	2017.0
47.00	2693.0
48.10	1377.0
49.00	8659.0
50.10	42320.0
51.10	12699.0
52.00	602.0
53.20	364.0
54.00	223.0
55.00	633.0
56.10	3088.0
57.00	5422.0
58.10	165.0
60.10	1917.0
61.00	10273.0
62.00	10278.0
63.00	8006.0
64.00	1568.0
65.00	1784.0
66.00	237.0
67.00	789.0
68.00	21496.0
69.00	22376.0
70.00	1712.0
71.00	131.0
72.00	1400.0
73.10	10014.0
74.10	37040.0
75.10	113144.0
76.00	9226.0
77.10	1145.0
78.00	907.0
78.90	6131.0
80.00	2005.0
80.90	6461.0
82.00	1408.0
83.10	170.0
86.10	527.0
86.90	9227.0
88.00	8465.0
90.90	876.0
92.00	7045.0
93.00	9955.0
94.00	26216.0
95.00	226688.0
96.00	13904.0
97.00	439.0
99.40	149.0
102.90	209.0
103.90	1042.0
104.90	444.0
105.90	999.0
106.80	308.0
107.90	181.0
109.00	109.0
110.00	255.0
111.10	125.0
112.10	195.0
113.00	166.0
114.80	250.0
116.00	950.0
117.00	1514.0
117.90	774.0
118.90	1446.0
122.00	235.0
123.00	143.0
124.00	136.0
125.70	145.0
126.80	127.0
127.90	965.0
128.80	428.0
129.80	640.0
131.00	306.0
132.10	115.0
135.00	448.0
135.80	200.0
136.90	343.0
139.80	222.0
140.90	2069.0
142.00	361.0
143.00	3029.0
143.80	232.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

145.00	1347.0
145.90	550.0
146.90	240.0
148.00	601.0
148.90	152.0
150.10	302.0
153.00	176.0
154.00	171.0
155.00	564.0
155.80	107.0
157.00	579.0
157.80	169.0
159.10	354.0
161.00	293.0
169.70	184.0
171.00	476.0
172.00	3013.0
174.00	220224.0
175.00	16104.0
176.00	210048.0
177.00	13891.0
178.00	621.0
204.40	114.0
262.20	109.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.00	1837.0
37.00	11006.0
38.10	9408.0
39.10	3875.0
40.00	1295.0
41.70	219.0
42.60	156.0
43.20	234.0
44.00	1617.0
45.00	2040.0
46.10	385.0
47.00	2678.0
48.10	1408.0
49.00	8868.0
50.10	42920.0
51.10	13271.0
52.00	495.0
53.20	358.0
54.00	169.0
55.00	639.0
56.00	3119.0
57.00	5712.0
58.00	220.0
60.00	2151.0
61.00	10720.0
62.00	10538.0
63.00	8267.0
64.00	1608.0
65.00	1841.0
66.00	277.0
67.00	680.0
68.00	21600.0
69.00	23120.0
70.00	1671.0
71.00	185.0
72.00	1516.0
73.10	10491.0
74.10	38592.0
75.00	114920.0
76.00	9889.0
77.10	1212.0
77.90	879.0
78.90	6216.0
80.10	2177.0
81.00	6235.0
82.00	1408.0
83.10	229.0
86.00	548.0
86.90	9542.0
88.00	8938.0
89.90	114.0
90.90	797.0
92.00	7028.0
93.00	10062.0
94.00	27248.0
95.00	235968.0
96.00	13927.0
97.00	415.0
99.40	188.0
102.90	214.0
103.90	1121.0
104.90	392.0
106.00	1033.0
106.90	283.0
107.90	199.0
109.00	146.0
110.00	270.0
111.10	130.0
112.00	230.0
113.00	186.0
114.90	267.0
115.90	990.0
116.90	1630.0
117.90	836.0
118.90	1352.0
122.00	199.0
122.80	147.0
124.00	203.0
125.80	146.0
128.00	967.0
128.80	406.0
129.80	688.0
130.10	634.0
131.00	307.0
135.00	415.0
135.80	262.0
136.90	377.0
139.80	283.0
140.90	2096.0
142.00	329.0
143.00	3268.0
143.80	306.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

145.00	1274.0
145.90	605.0
146.90	189.0
148.00	611.0
148.90	251.0
150.00	295.0
152.90	178.0
154.00	183.0
155.10	572.0
155.90	162.0
157.00	512.0
157.80	195.0
159.00	385.0
160.90	342.0
169.70	197.0
170.90	508.0
172.00	2960.0
174.00	231232.0
175.00	16928.0
176.00	220992.0
177.00	14524.0
178.00	592.0
259.30	128.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
36.10	1798.0
37.00	10402.0
38.10	8409.0
39.10	3380.0
40.00	1110.0
41.70	223.0
42.50	152.0
43.10	211.0
44.00	1469.0
45.00	1902.0
46.00	305.0
47.00	2466.0
48.00	1361.0
49.00	8186.0
50.00	38832.0
51.10	12055.0
52.00	388.0
53.20	368.0
54.10	130.0
55.00	573.0
56.00	2868.0
57.00	5321.0
58.00	261.0
60.00	2189.0
61.00	9935.0
62.00	9561.0
63.00	7992.0
64.00	1474.0
65.00	1670.0
66.00	243.0
67.00	614.0
68.00	19872.0
69.00	21200.0
70.00	1558.0
71.10	198.0
72.00	1337.0
73.10	9909.0
74.10	36776.0
75.00	106200.0
76.00	9003.0
77.10	1084.0
77.90	793.0
79.00	5526.0
80.00	1992.0
81.00	5761.0
82.00	1343.0
83.10	218.0
86.00	563.0
87.00	9293.0
88.00	8321.0
89.90	149.0
90.90	656.0
92.00	6267.0
93.00	8824.0
94.10	25280.0
95.00	221056.0
96.10	12734.0
97.00	387.0
99.40	145.0
102.90	154.0
103.90	1019.0
104.90	315.0
106.00	1007.0
107.00	245.0
108.00	185.0
109.00	149.0
109.90	243.0
111.10	134.0
112.00	208.0
113.00	195.0
114.90	284.0
115.90	899.0
116.90	1669.0
117.90	838.0
118.90	1249.0
121.20	151.0
122.00	116.0
123.10	117.0
124.00	240.0
124.80	107.0
125.80	127.0
126.90	109.0
128.00	827.0
129.00	395.0
129.80	721.0
130.90	283.0
135.00	395.0
135.80	258.0
136.90	406.0
139.90	325.0
140.90	1864.0
142.00	311.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

143.00	3224.0
143.80	307.0
145.00	955.0
145.90	615.0
147.90	563.0
148.90	281.0
150.00	299.0
152.90	178.0
154.00	204.0
155.10	522.0
155.90	206.0
156.80	444.0
157.80	199.0
159.00	350.0
160.90	391.0
169.00	107.0
169.70	147.0
170.90	453.0
172.00	2602.0
174.00	218688.0
175.00	16159.0
176.00	210304.0
177.00	13419.0
178.00	522.0
232.90	112.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33

m/z	Abundance
35.90	170.0
36.40	189.0
38.10	197.0
38.90	162.0
39.90	824.0
41.50	198.0
42.20	141.0
43.30	141.0
44.10	800.0
46.30	168.0
46.90	101.0
48.10	155.0
49.30	121.0
50.60	148.0
51.80	138.0
52.80	110.0
53.50	159.0
54.00	193.0
55.10	138.0
56.10	112.0
58.00	149.0
59.40	125.0
61.00	168.0
63.10	112.0
65.20	106.0
68.00	114.0
70.30	104.0
76.00	181.0
77.10	106.0
78.10	108.0
81.80	109.0
135.70	141.0
165.70	128.0
193.50	116.0

Instrument :
MSVOA_V
ClientSampleId :
BFB33