

Data Path : Z:\VOASRV\HPCHEM1\MSVOA V\DATA\VV111820\
 Data File : VV019398.D
 Acq On : 18 Nov 2020 17:08
 Operator : SY/MD
 Sample : VSTDCCC0.5EC
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VSTD0.5308

Quant Time: Nov 19 07:46:00 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMV111820SIM.M
 Quant Title : TRACE VOA SOM01.0
 QLast Update : Thu Nov 19 07:44:21 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	5.64	114	5712	0.50	ug/L	0.00
5) Chlorobenzene-d5	8.88	117	5368	0.50	ug/L	0.00
11) 1,4-Dichlorobenzene-d4	11.28	152	2860	0.50	ug/L	0.00

System Monitoring Compounds

2) Vinyl Chloride-d3	1.32	65	4186	0.51	ug/L	0.00
Spiked Amount	0.500	Range	40 - 130	Recovery	=	102.00%
4) 1,2-Dichloroethane-d4	5.04	65	2540	0.53	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	106.00%
7) 1,2-Dichloropropane-d6	6.09	67	2372	0.53	ug/L	0.00
Spiked Amount	0.500	Range	60 - 140	Recovery	=	106.00%
8) Toluene-d8	7.33	98	6331	0.49	ug/L	0.00
Spiked Amount	0.500	Range	70 - 130	Recovery	=	98.00%
10) 1,1,2,2-Tetrachloroethane-	10.23	84	1226	0.51	ug/L	0.00
Spiked Amount	0.500	Range	65 - 120	Recovery	=	102.00%

Target Compounds


					Qvalue
3) Vinyl chloride	1.32	62	3829	0.518 ug/L	99
6) Trichloroethene	5.93	95	2395	0.536 ug/L	97
9) 1,2-Dibromoethane	8.37	107	1352	0.531 ug/L	94
12) 1,2,3-Trichloropropane	10.28	75	1127	0.537 ug/L	98
13) 1,2-Dibromo-3-chloropropan	12.44	75	181	0.533 ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA V\DATA\VV111820\
Data File : VV019398.D
Acq On : 18 Nov 2020 17:08
Operator : SY/MD
Sample : VSTDCCC0.5EC
Misc : 25.0mL/MSVOA V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VSTD0.5308

Quant Time: Nov 19 07:46:00 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_V\METHOD\SFAMV111820SIM.M
Quant Title : TRACE VOA SOM01.0
QLast Update : Thu Nov 19 07:44:21 2020
Response via : Initial Calibration

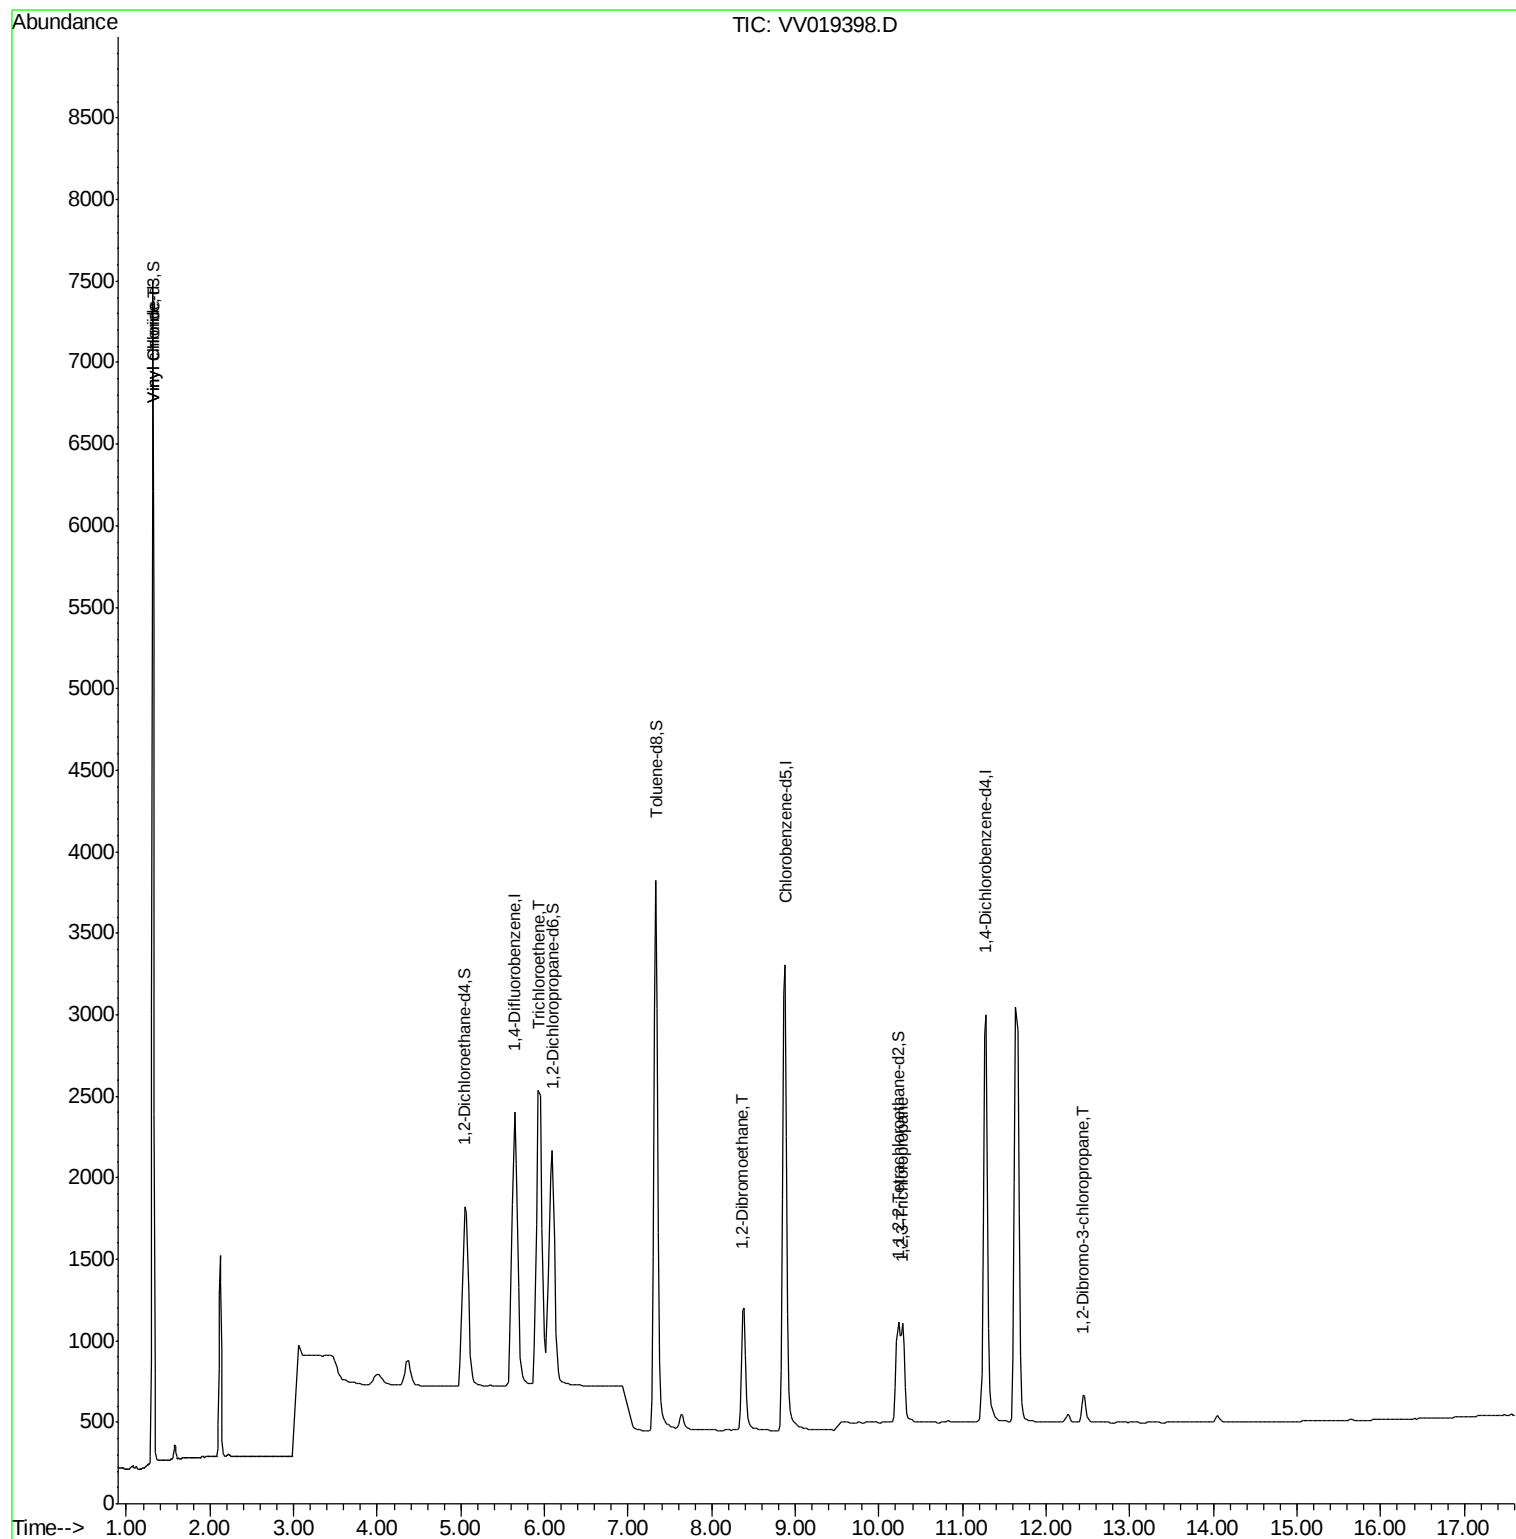

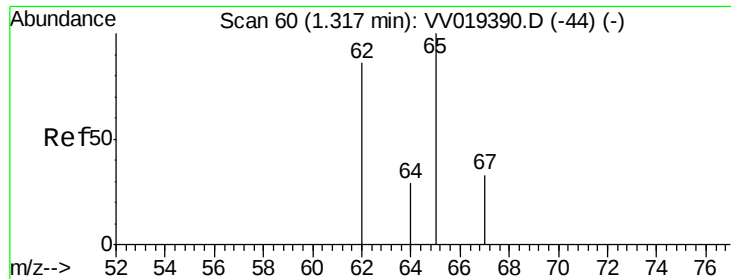

#3

Vinyl chloride

Concen: 0.518 ug/L

RT: 1.32 min Scan# 60

Delta R.T. -0.00 min

Lab File: VV019398.D

Acq: 18 Nov 2020 17:08

Instrument :

MSVOA_V

ClientSampleId :





VSTD0.5308

Tot Ion: 62 Resp: 3829

Ion Ratio Lower Upper

62 100

64 35.2 25.1 46.7

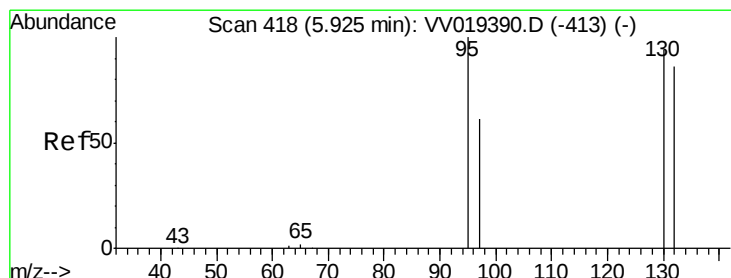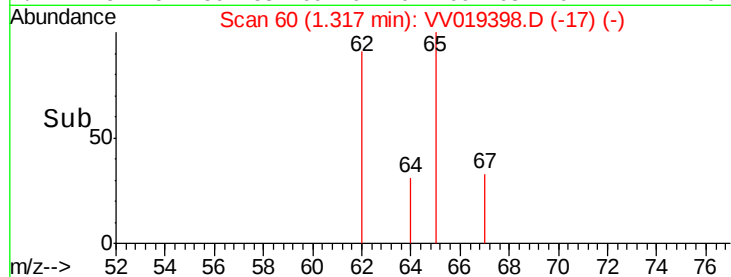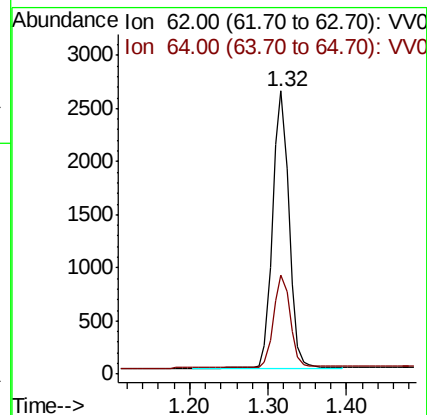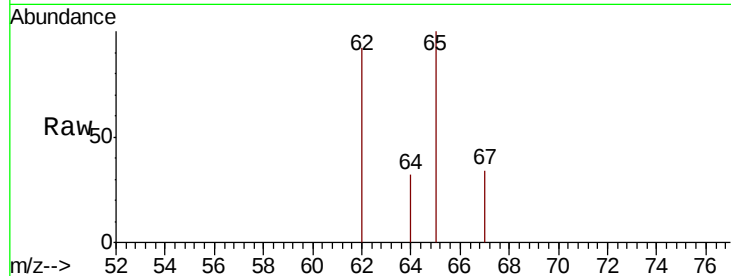

#6

Trichloroethene

Concen: 0.536 ug/L

RT: 5.93 min Scan# 418

Delta R.T. -0.00 min

Lab File: VV019398.D

Acq: 18 Nov 2020 17:08

Tgt Ion: 95 Resp: 2395




Ion Ratio Lower Upper


95 100

97 66.5 45.6 84.6

132 89.7 61.0 113.2

130 96.8 65.9 122.3

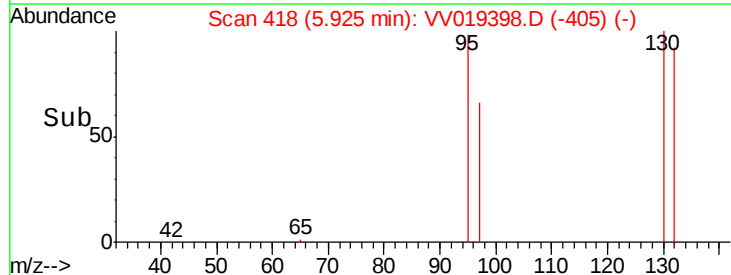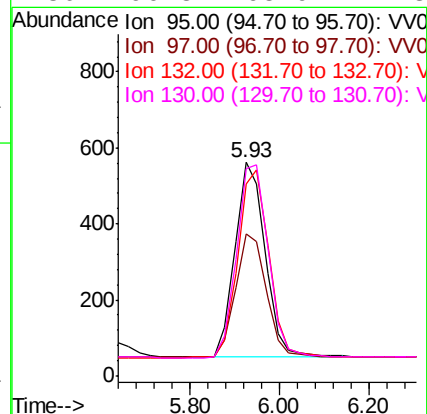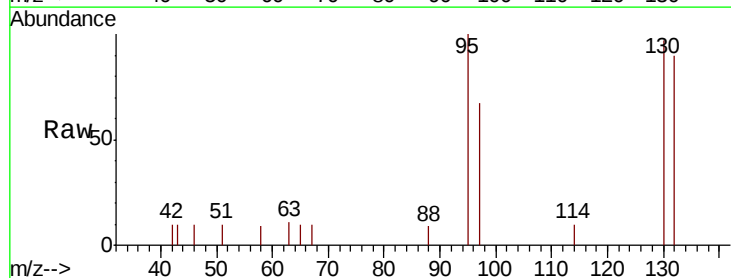

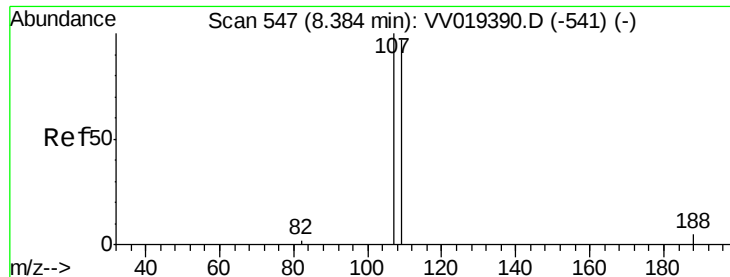

#9

1,2-Dibromoethane

Concen: 0.531 ug/L

RT: 8.37 min Scan# 546

Delta R.T. -0.02 min

Lab File: VV019398.D

Acq: 18 Nov 2020 17:08

Instrument :

MSVOA_V

ClientSampled :

VSTD0.5308


Tot Ion:107 Resp: 1352

Ion Ratio Lower Upper

107 100

109 91.7 68.5 127.1



188 14.7 13.9 20.9

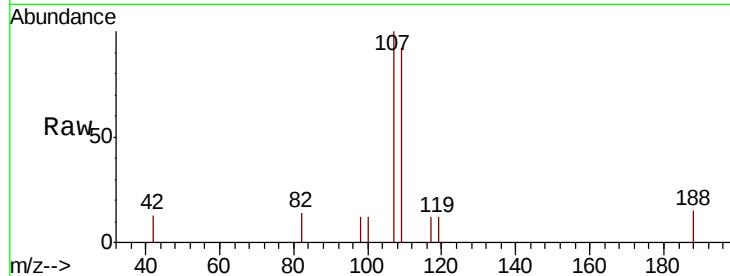


Abundance Ion 107.00 (106.70 to 107.70): V

Ion 109.00 (108.70 to 109.70): V

Ion 188.00 (187.70 to 188.70): V

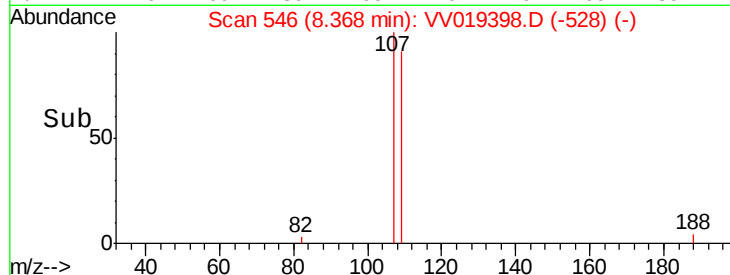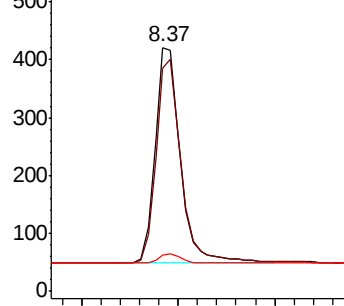

Time-->

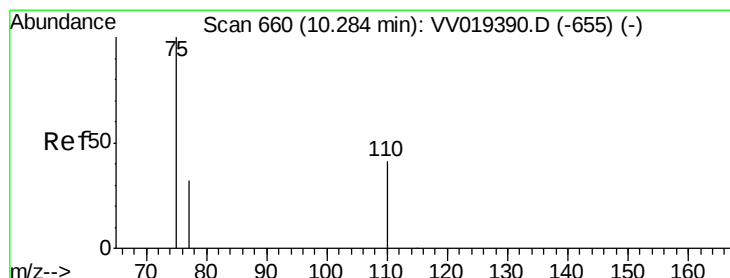

#12

1,2,3-Trichloropropane

Concen: 0.537 ug/L

RT: 10.28 min Scan# 660

Delta R.T. -0.00 min

Lab File: VV019398.D

Acq: 18 Nov 2020 17:08


Tgt Ion: 75 Resp: 1127

Ion Ratio Lower Upper

75 100

110 44.9 34.5 51.7



77 32.2 25.7 38.5

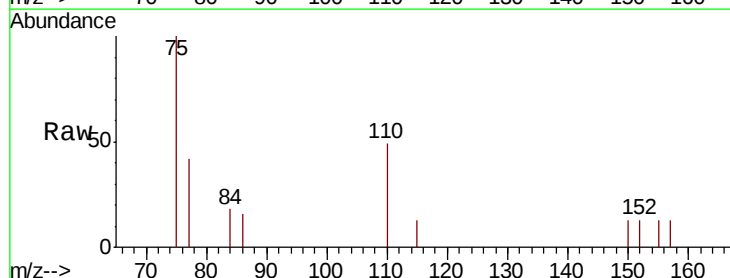


Abundance Ion 75.00 (74.70 to 75.70): VV0

Ion 110.00 (109.70 to 110.70): V

Ion 77.00 (76.70 to 77.70): VV0

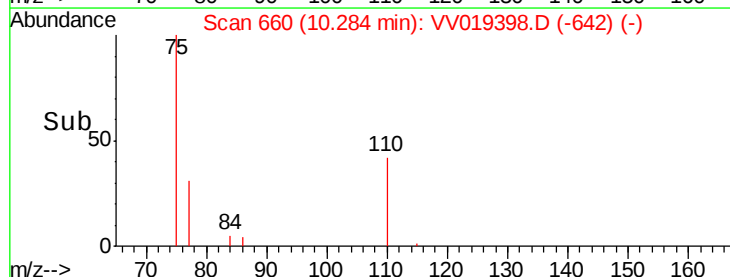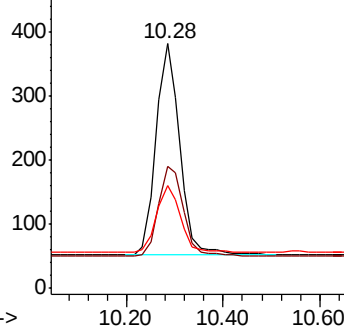

Time-->

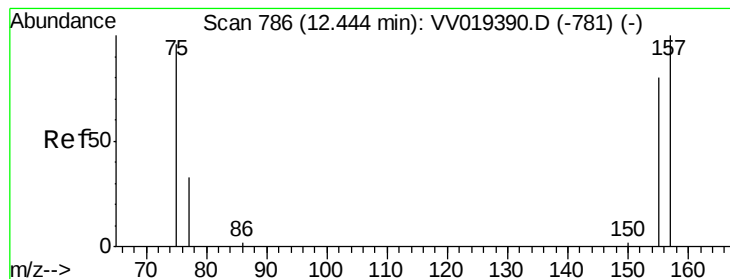

#13

1,2-Dibromo-3-chloropropane

Concen: 0.533 ug/L

RT: 12.44 min Scan# 786

Delta R.T. -0.00 min

Lab File: VV019398.D

Acq: 18 Nov 2020 17:08

Instrument :

MSVOA_V

ClientSampleId :

VSTD0.5308



Tot Ion: 75 Resp: 181

Ion Ratio Lower Upper

75 100

157 100.0 79.2 118.8

155 89.4 71.0 106.6

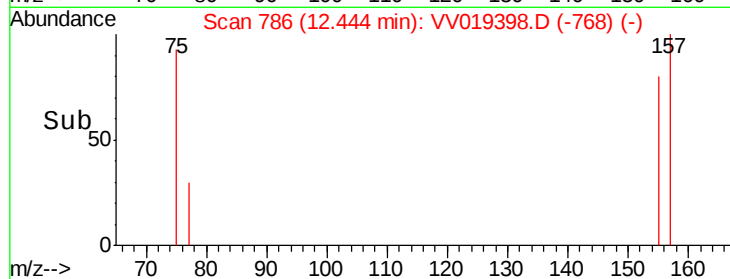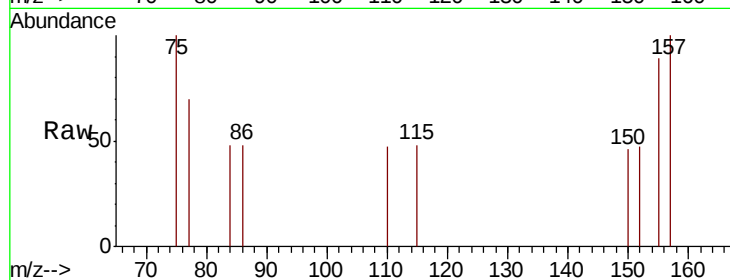

Abundance Ion 75.00 (74.70 to 75.70): VV019398.D (-768) (-)

Ion 157.00 (156.70 to 157.70): VV019398.D (-768) (-)

Ion 155.00 (154.70 to 155.70): VV019398.D (-768) (-)

