


Data Path : Z:\voasrv\HPCHEM1\MSVOA V\Data\VV111820\
 Data File : VV019387.D
 Acq On : 18 Nov 2020 08:37
 Operator : SY/MD
 Sample : BFB63
 Misc : 25.0mL/MSVOA V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB63

Integration File: rteint.p

Method : Z:\VOASRV\HPCHEM1\MSVOA_V\METHOD\SFAMV111820SIM.M
 Title : TRACE VOA SOM01.0
 Last Update : Thu Nov 19 07:44:21 2020

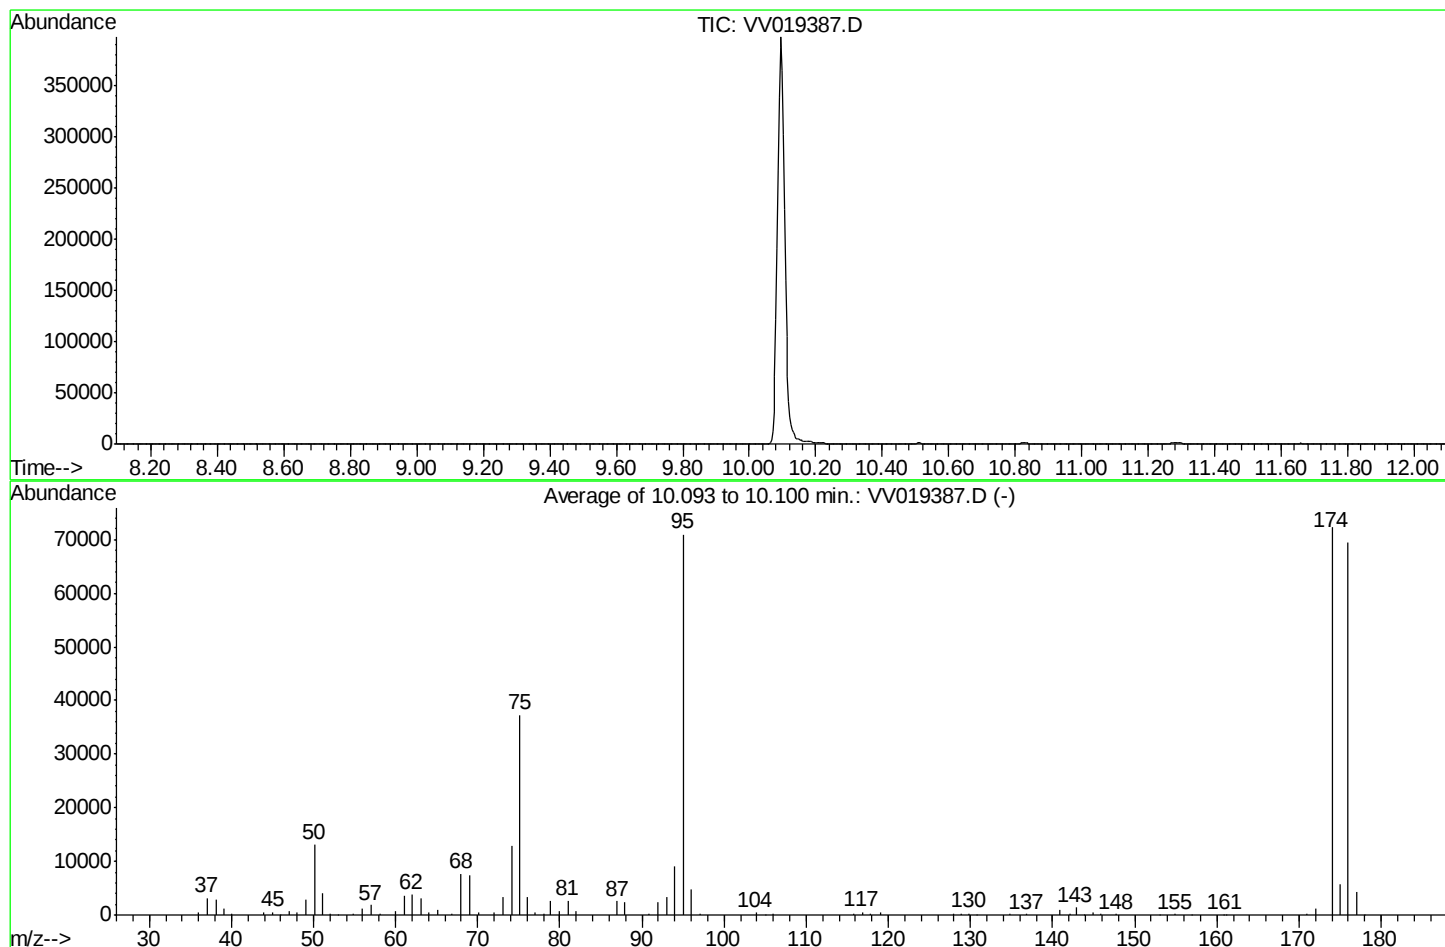

AutoFind: Scans 2800, 2801, 2802; Background Corrected with Scan 2788

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.4	13059	PASS
75	95	30	80	52.5	37250	PASS
95	95	100	100	100.0	70938	PASS
96	95	5	9	6.7	4766	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	101.9	72301	PASS
175	174	5	9	7.9	5696	PASS
176	174	95	101	95.9	69360	PASS
177	176	5	9	6.4	4406	PASS

m/z	Abundance
36.00	542.0
37.00	3318.0
38.10	2836.0
39.00	1174.0
40.00	124.0
44.00	550.0
45.00	579.0
45.90	153.0
47.00	536.0
48.00	386.0
49.00	2793.0
50.10	13590.0
51.00	4332.0
52.10	226.0
54.90	222.0
56.00	1188.0
57.00	2049.0
58.10	117.0
60.00	731.0
61.00	3765.0
62.00	3780.0
63.10	3255.0
64.00	584.0
65.10	925.0
66.90	200.0
68.00	7690.0
69.00	7469.0
70.10	514.0
71.90	504.0
73.00	3420.0
74.10	13280.0
75.10	38264.0
76.00	3516.0
76.90	498.0
78.00	250.0
78.90	2644.0
80.00	686.0
81.00	2793.0
81.90	666.0
87.00	2539.0
87.90	2482.0
90.80	319.0
92.00	2407.0
93.00	3585.0
94.00	9149.0
95.00	71960.0
96.00	5013.0
97.10	179.0
103.90	402.0
105.90	352.0
115.90	314.0
116.80	587.0
117.80	327.0
119.00	496.0
127.90	262.0
128.80	159.0
129.80	306.0
134.90	163.0
136.90	204.0
140.90	913.0
142.10	140.0
142.90	1335.0
143.90	102.0
144.90	495.0
145.90	182.0
147.80	218.0
153.10	129.0
154.90	208.0
156.90	149.0
160.80	106.0
161.10	129.0
170.90	240.0
172.00	1100.0
174.00	72216.0
175.00	5669.0
176.00	68576.0
177.00	4470.0
177.90	139.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	512.0
37.00	3329.0
38.10	2841.0
39.00	1239.0
40.00	128.0
44.00	584.0
45.10	574.0
45.90	143.0
47.00	664.0
48.00	410.0
49.00	2929.0
50.10	13543.0
51.10	4235.0
52.00	269.0
52.90	107.0
54.90	227.0
56.00	1173.0
57.00	1950.0
58.10	136.0
60.00	744.0
61.00	3636.0
62.00	3992.0
63.10	3330.0
64.00	551.0
65.00	958.0
66.80	196.0
68.00	8011.0
69.00	7744.0
70.10	558.0
71.90	507.0
73.00	3442.0
74.10	13291.0
75.10	38536.0
76.00	3524.0
76.90	460.0
78.10	208.0
78.90	2621.0
80.00	778.0
81.00	2787.0
81.90	738.0
87.00	2673.0
88.00	2382.0
90.90	358.0
92.00	2408.0
93.00	3522.0
94.00	9308.0
95.10	73520.0
96.00	4979.0
97.00	144.0
103.90	458.0
105.00	104.0
105.90	315.0
115.80	327.0
116.90	620.0
117.80	369.0
119.00	503.0
127.90	288.0
128.80	155.0
129.90	332.0
134.80	200.0
136.90	216.0
140.90	965.0
142.10	160.0
142.90	1407.0
144.90	496.0
145.90	191.0
147.80	209.0
153.00	124.0
154.90	229.0
156.90	124.0
161.10	118.0
170.90	213.0
172.00	1266.0
174.00	74896.0
175.00	5927.0
176.00	71904.0
177.00	4488.0
178.00	111.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
36.00	489.0
37.10	2965.0
38.10	2705.0
39.10	1190.0
40.00	151.0
44.00	541.0
45.10	507.0
47.00	682.0
48.00	382.0
49.00	2646.0
50.10	12044.0
51.10	3647.0
52.10	293.0
52.90	107.0
54.90	230.0
56.00	1037.0
57.00	1653.0
58.00	152.0
60.00	686.0
61.00	3207.0
62.00	3632.0
63.10	3096.0
64.00	428.0
65.00	863.0
66.80	171.0
68.00	7268.0
69.00	6999.0
70.10	528.0
71.90	430.0
73.00	3066.0
74.10	11955.0
75.10	34952.0
76.00	3090.0
76.90	389.0
78.90	2381.0
80.00	727.0
81.00	2487.0
82.00	704.0
87.00	2597.0
88.00	2112.0
90.90	368.0
92.00	2144.0
93.00	3112.0
94.00	8469.0
95.10	67336.0
96.00	4308.0
97.00	105.0
103.90	411.0
105.00	109.0
105.90	296.0
115.80	268.0
116.90	555.0
117.80	350.0
119.00	432.0
127.90	296.0
128.80	130.0
129.90	341.0
130.80	108.0
134.80	196.0
136.80	201.0
140.90	874.0
142.10	160.0
142.90	1301.0
145.00	455.0
145.90	167.0
147.70	176.0
153.00	112.0
155.00	219.0
156.80	103.0
170.90	180.0
172.00	1230.0
174.00	69792.0
175.00	5493.0
176.00	67600.0
177.00	4260.0
178.00	103.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63

m/z	Abundance
43.90	143.0

Instrument :
MSVOA_V
ClientSampleId :
BFB63