




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029109.D
 Acq On : 18 Nov 2022 11:36
 Operator : SY/MD
 Sample : N5604-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:33:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 04:35:43 2022
 Response via : Initial Calibration

Reviewed By :Krupa Patel 11/20/2022
 Supervised By :Mahesh Dadoda 11/20/2022

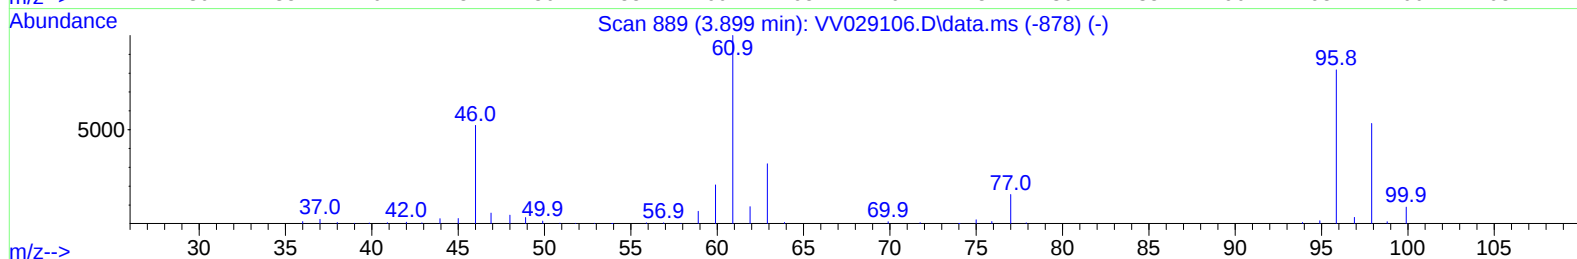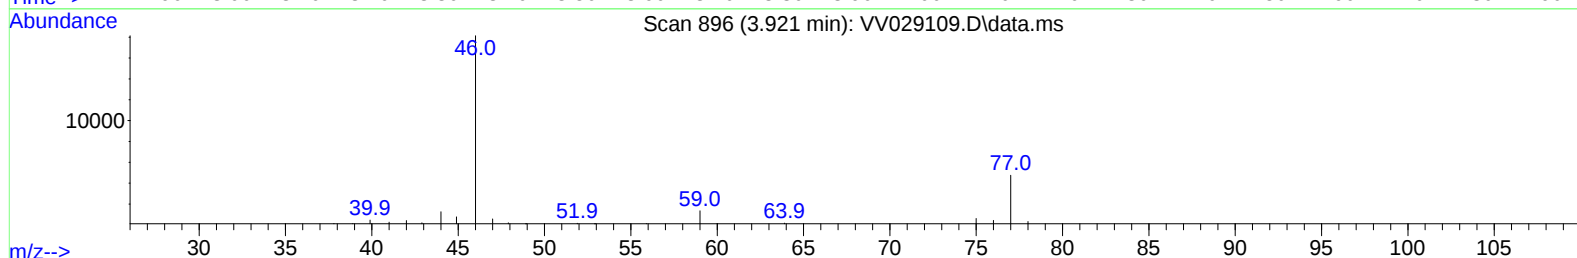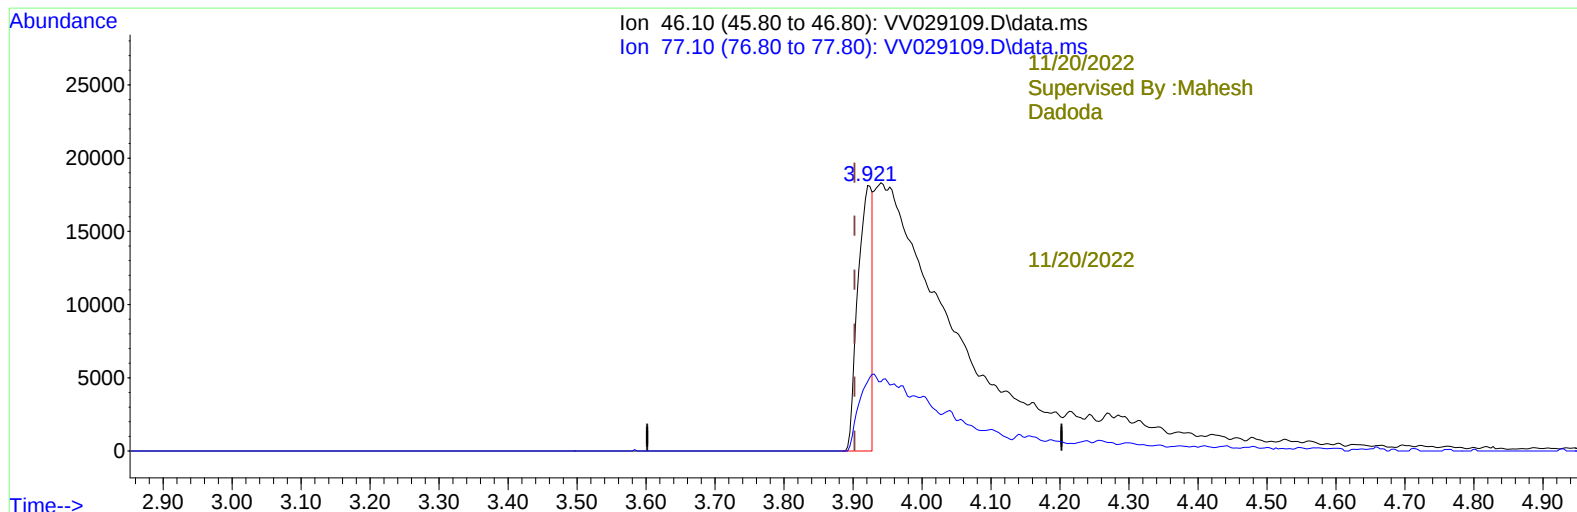

TIC: VV029109.D\data.ms

(20) 2-Butanone-d5 (S)

3.921min (+ 0.019) 7.79 ug/L

response 26080

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.70	41.59#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029109.D
 Acq On : 18 Nov 2022 11:36
 Operator : SY/MD
 Sample : N5604-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/20/2022
 Supervised By :Mahesh Dadoda 11/20/2022

Quant Time: Nov 18 23:33:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 04:35:43 2022
 Response via : Initial Calibration

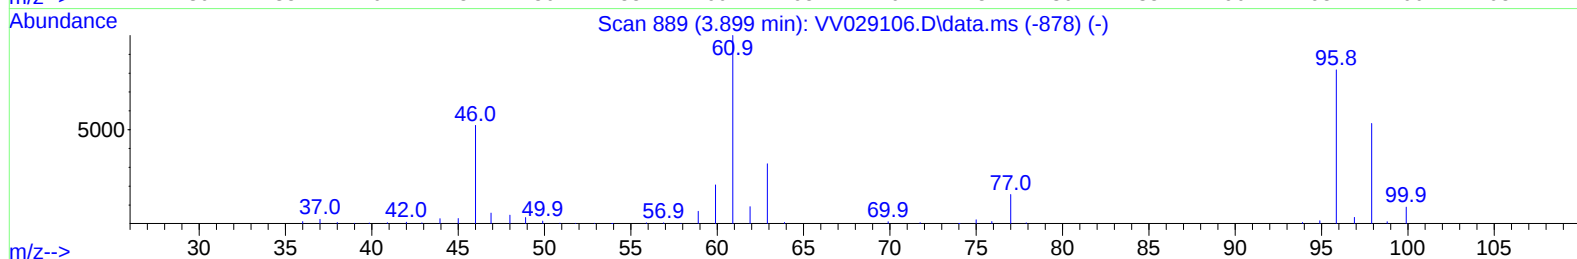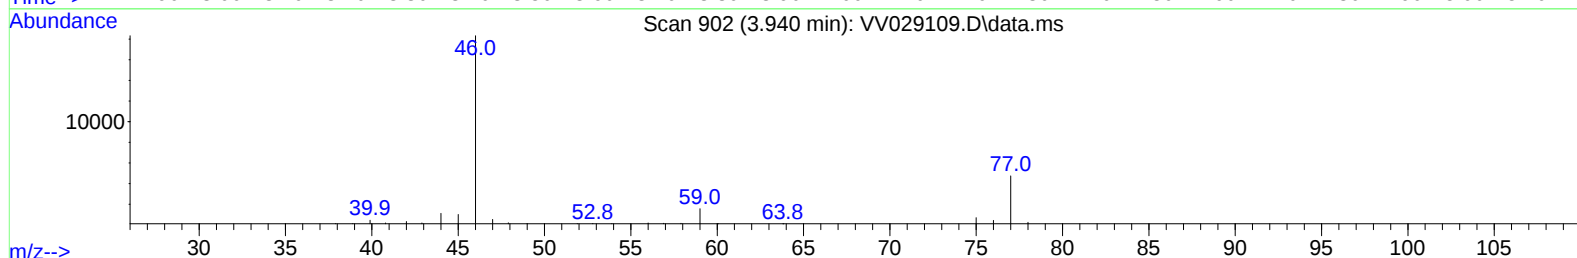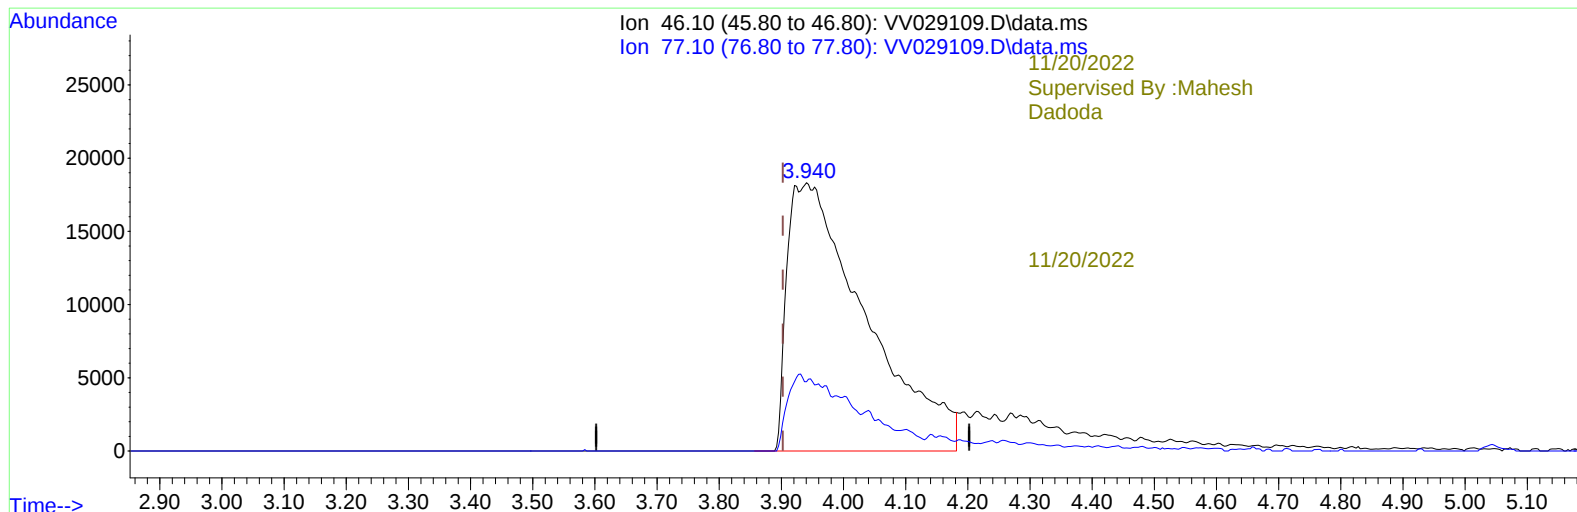

TIC: VV029109.D\data.ms

(20) 2-Butanone-d5 (S)

3.940min (+ 0.038) 47.93 ug/L m

response 160398

Ion	Exp%	Act%
46.10	100.00	100.00
77.10	24.70	6.76#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
 Data File : VV029109.D
 Acq On : 18 Nov 2022 11:36
 Operator : SY/MD
 Sample : N5604-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 11/20/2022
 Supervised By :Mahesh Dadoda 11/20/2022

Quant Time: Nov 18 23:33:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 04:35:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	327923	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	300823	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	138981	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	122213	6.113	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery = 122.200%			
7) Chloroethane-d5	1.568	69	93954	5.346	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery = 107.000%			
11) 1,1-Dichloroethene-d2	2.104	63	156247	4.289	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery = 85.800%			
20) 2-Butanone-d5	3.940	46	160398m	47.929	ug/L	0.04
Spiked Amount	50.000	Range 40 - 130	Recovery = 95.860%			
24) Chloroform-d	4.342	84	187075	4.558	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery = 91.200%			
26) 1,2-Dichloroethane-d4	5.027	65	88726	4.805	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery = 96.000%			
32) Benzene-d6	5.046	84	420700	4.685	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery = 93.800%			
36) 1,2-Dichloropropane-d6	6.066	67	122241	4.875	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery = 97.600%			
41) Toluene-d8	7.310	98	370713	4.586	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery = 91.800%			
43) trans-1,3-Dichloroprop...	7.622	79	35692	4.365	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery = 87.200%			
46) 2-Hexanone-d5	8.091	63	146023	41.833	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery = 83.660%			
56) 1,1,2,2-Tetrachloroeth...	10.210	84	80878	4.653	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery = 93.000%			
66) 1,2-Dichlorobenzene-d4	11.615	152	125687	5.055	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery = 101.000%			
Target Compounds						
16) Methylene chloride	2.506	84	9798	0.382	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029109.D
Acq On : 18 Nov 2022 11:36
Operator : SY/MD
Sample : N5604-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Nov 18 23:33:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 04:35:43 2022
Response via : Initial Calibration

Reviewed By :Krupa Patel 11/20/2022
Supervised By :Mahesh Dadoda 11/20/2022

