

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111822\
 Data File : VW029112.D
 Acq On : 18 Nov 2022 12:46
 Operator : SY/MD
 Sample : N5687-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCD2

Quant Time: Nov 18 23:33:38 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 04:35:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.616	114	269653	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	233659	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	114922	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	76625	4.661	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	93.200%	
7) Chloroethane-d5	1.564	69	67882	4.697	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	94.000%	
11) 1,1-Dichloroethene-d2	2.105	63	108401	3.618	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	72.400%	
20) 2-Butanone-d5	3.908	46	156932	57.027	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	114.060%	
24) Chloroform-d	4.346	84	168464	4.991	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.800%	
26) 1,2-Dichloroethane-d4	5.031	65	80887	5.327	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.600%	
32) Benzene-d6	5.047	84	348134	4.992	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	99.800%	
36) 1,2-Dichloropropane-d6	6.066	67	108897	5.592	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	111.800%	
41) Toluene-d8	7.313	98	302455	4.818	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	96.400%	
43) trans-1,3-Dichloroprop...	7.622	79	33225	5.231	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	104.600%	
46) 2-Hexanone-d5	8.088	63	153888	56.759	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	113.520%	
56) 1,1,2,2-Tetrachloroeth...	10.210	84	80998	5.999	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	120.000%	
66) 1,2-Dichlorobenzene-d4	11.615	152	114721	5.580	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	111.600%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.240	50	4476	0.240	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029112.D
Acq On : 18 Nov 2022 12:46
Operator : SY/MD
Sample : N5687-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCD2

Quant Time: Nov 18 23:33:38 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 04:35:43 2022
Response via : Initial Calibration

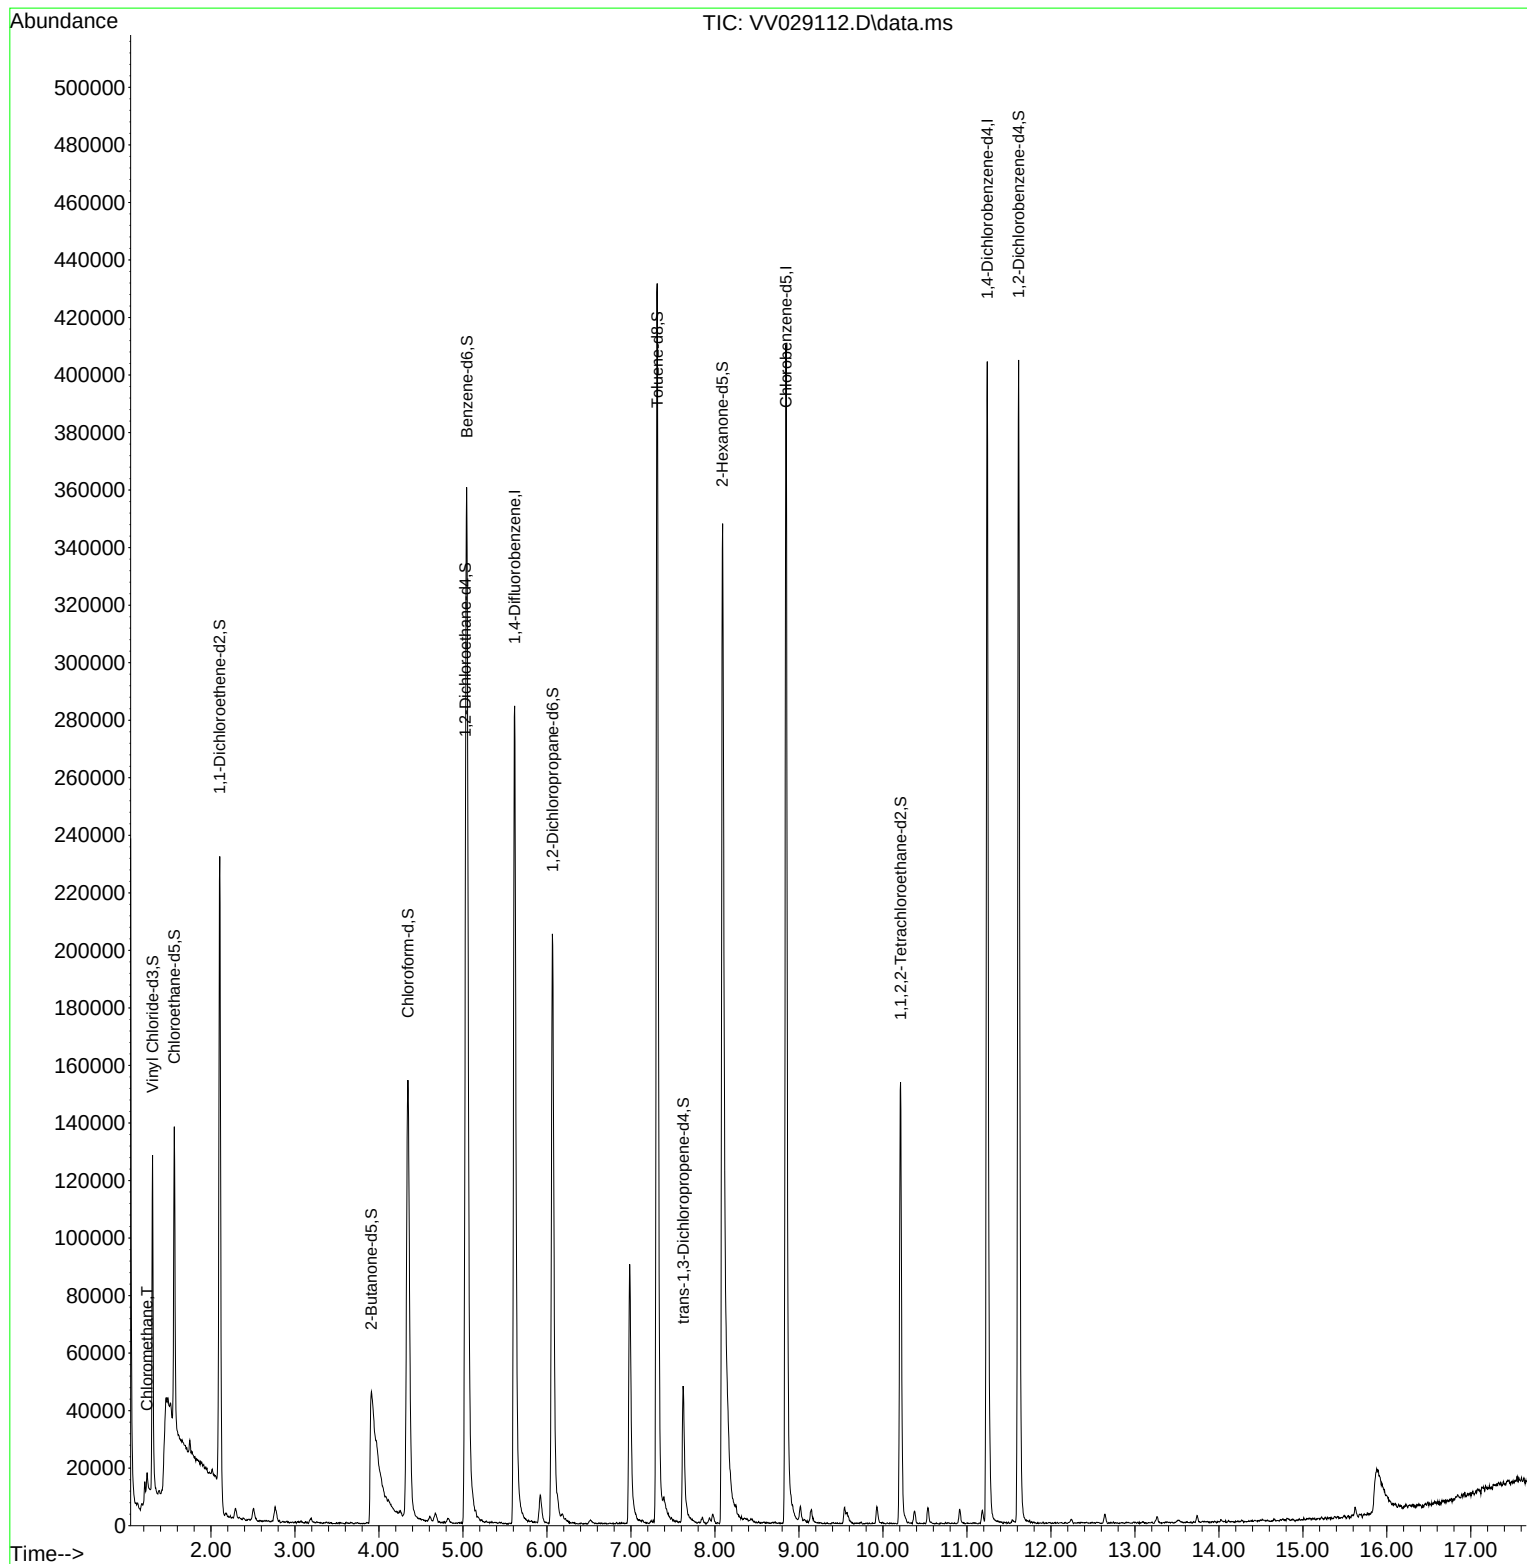

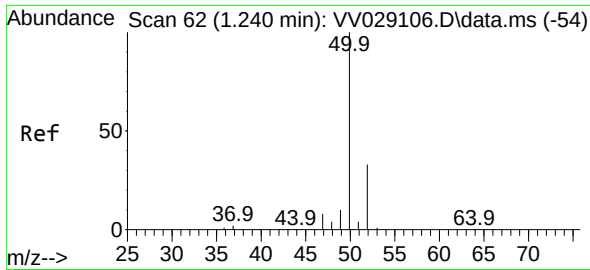

#3
 Chloromethane
 Concen: 0.240 ug/L
 RT: 1.240 min Scan# 61
 Delta R.T. -0.000 min
 Lab File: VV029112.D
 Acq: 18 Nov 2022 12:46

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCD2

Tgt Ion: 50 Resp: 4476
 Ion Ratio Lower Upper
 50 100
 52 34.3 23.7 43.9

