

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VW111822\
 Data File : VW029119.D
 Acq On : 18 Nov 2022 15:35
 Operator : SY/MD
 Sample : N5687-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGCD9

Quant Time: Nov 18 23:34:31 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Nov 18 04:35:43 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	278120	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	256106	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.242	152	112850	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.307	65	73955	4.362	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	87.200%	
7) Chloroethane-d5	1.568	69	67329	4.517	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	90.400%	
11) 1,1-Dichloroethene-d2	2.105	63	103408	3.347	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	67.000%	
20) 2-Butanone-d5	3.892	46	194573	68.553	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	137.100%#	
24) Chloroform-d	4.342	84	169833	4.879	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	97.600%	
26) 1,2-Dichloroethane-d4	5.030	65	83286	5.318	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	106.400%	
32) Benzene-d6	5.047	84	353468	4.624	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	92.400%	
36) 1,2-Dichloropropane-d6	6.066	67	109674	5.138	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	102.800%	
41) Toluene-d8	7.310	98	312671	4.544	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	90.800%	
43) trans-1,3-Dichloroprop...	7.622	79	34342	4.933	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	98.600%	
46) 2-Hexanone-d5	8.088	63	155429	52.303	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	104.600%	
56) 1,1,2,2-Tetrachloroeth...	10.207	84	81352	5.497	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	110.000%	
66) 1,2-Dichlorobenzene-d4	11.615	152	110041	5.450	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	109.000%	
Target Compounds						
					Qvalue	
3) Chloromethane	1.240	50	6184	0.321	ug/L	96
55) Styrene	9.561	104	35204	0.631	ug/L	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV111822\
Data File : VV029119.D
Acq On : 18 Nov 2022 15:35
Operator : SY/MD
Sample : N5687-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGCD9

Quant Time: Nov 18 23:34:31 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR111122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Nov 18 04:35:43 2022
Response via : Initial Calibration

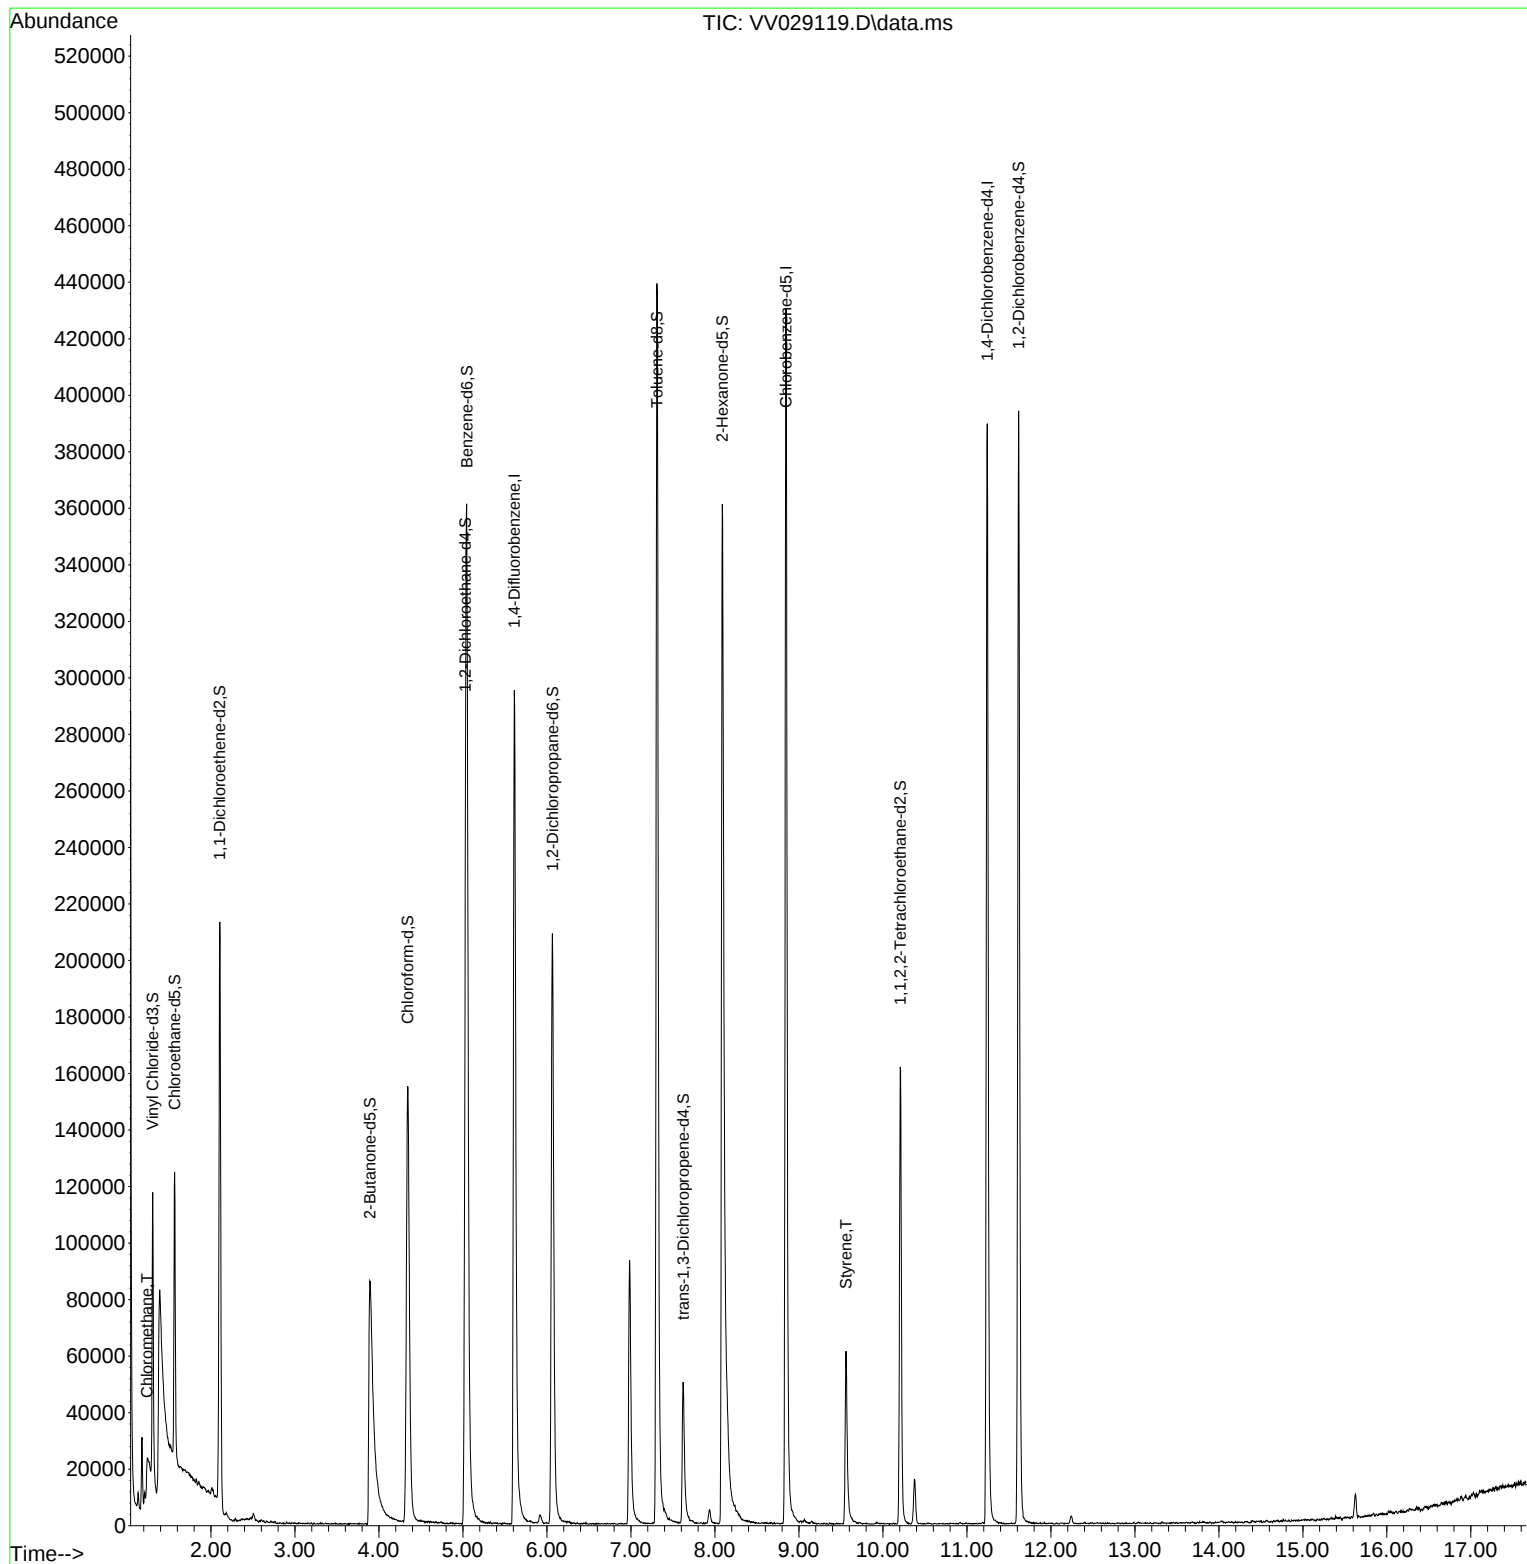

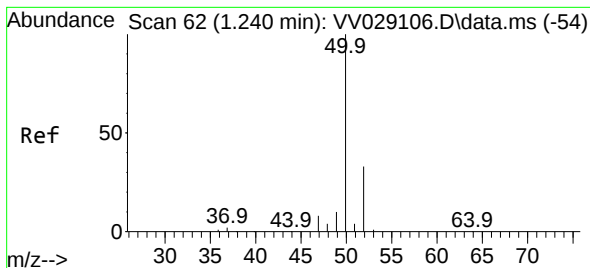

#3

Chloromethane

Concen: 0.321 ug/L

RT: 1.240 min Scan# 61

Delta R.T. -0.000 min

Lab File: VV029119.D

Acq: 18 Nov 2022 15:35

Instrument :

MSVOA_V

ClientSampleId :





BGCD9

Tgt Ion: 50 Resp: 6184

Ion Ratio Lower Upper

50 100

52 31.4 23.7 43.9

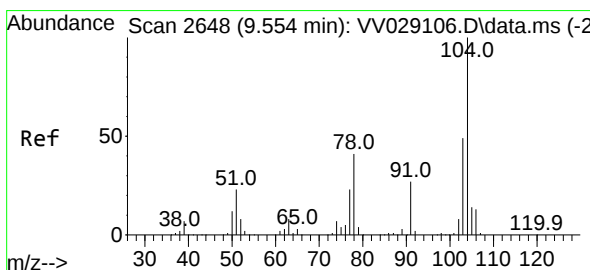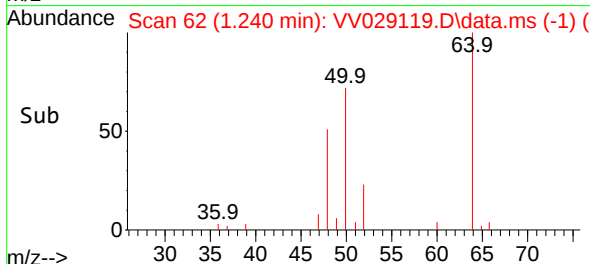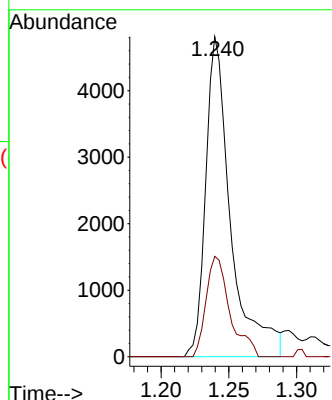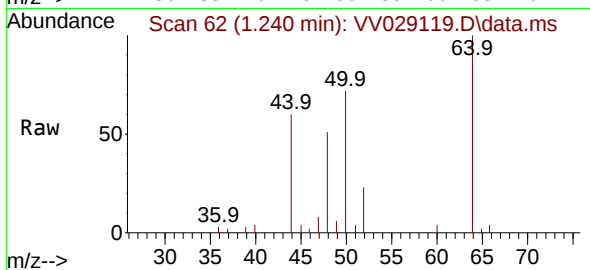

#55

Styrene

Concen: 0.631 ug/L

RT: 9.561 min Scan# 2650

Delta R.T. 0.006 min

Lab File: VV029119.D

Acq: 18 Nov 2022 15:35

Tgt Ion: 104 Resp: 35204

Ion Ratio Lower Upper

104 100

78 39.0 30.1 55.9

